



IBM System x

IBM Hardware Management Pack for  
Microsoft System Center Operations Manager  
Installation and User's Guide

*Version 5.5*







IBM System x

IBM Hardware Management Pack for  
Microsoft System Center Operations Manager  
Installation and User's Guide

*Version 5.5*

**Note**

Before using this information and the product it supports, read the information in “Notices” on page 137.

**Edition Notice**

This edition applies to the IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 and to all subsequent releases and modifications until otherwise indicated in new editions.

© Copyright IBM Corporation 2014.

US Government Users Restricted Rights – Use, duplication or disclosure restricted by GSA ADP Schedule Contract with IBM Corp.

# Contents

<b>Figures</b> . . . . .	<b>v</b>
--------------------------	----------

<b>Tables</b> . . . . .	<b>vii</b>
-------------------------	------------

<b>About this publication</b> . . . . .	<b>ix</b>
Conventions and terminology . . . . .	ix

<b>Information resources</b> . . . . .	<b>xi</b>
PDF files . . . . .	xi
World Wide Web resources . . . . .	xi

<b>Chapter 1. IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5</b> . . . . .	<b>1</b>
Key features . . . . .	1
Premium features. . . . .	1
Trial license support . . . . .	2

<b>Chapter 2. Technical overview</b> . . . . .	<b>3</b>
How the IBM Hardware Management Pack supports IBM systems . . . . .	4
Management concepts . . . . .	4

<b>Chapter 3. Supported configurations</b> . . . . .	<b>5</b>
Supported systems . . . . .	5
Supported IBM servers . . . . .	5
Supported IBM BladeCenter chassis . . . . .	7
Supported IBM Flex System chassis. . . . .	7
Agentless support . . . . .	7
Supported configurations of management servers. . . . .	10
Supported versions of Microsoft System Center Operations Manager for management servers . . . . .	10
Prerequisites for Hardware Failure Management . . . . .	10
Supported operating systems for management servers . . . . .	10
Additional configuration requirements for management servers . . . . .	11
Supported configurations and requirements for a managed system. . . . .	11
Supported operating systems for managed systems. . . . .	11
Supported versions of IBM Systems Director Agent . . . . .	12
Supported configurations of IBM Systems Director Agent . . . . .	12
Supported configurations of managed systems with BMC or IPMI . . . . .	13
Supported configurations of managed systems with Remote Supervisor Adapter-II . . . . .	13
Supported configurations of managed systems with ServeRAID-MR or MegaRAID . . . . .	14
Supported configurations of managed systems with ServeRAID-BR/IR or Integrated RAID . . . . .	14

Supported configurations of managed systems with ServeRAID versions 8x/7x/6x . . . . .	15
Supported configurations of managed systems with Power Monitoring . . . . .	15

<b>Chapter 4. Installing the IBM Hardware Management Pack and other components</b> . . . . .	<b>17</b>
Overview of the installation process . . . . .	17
Installation requirements for the IBM Hardware Management Pack . . . . .	18
Installing the IBM Hardware Management Pack . . . . .	19
Steps for installing the IBM Hardware Management Pack . . . . .	20
IBM Hardware Management Packs . . . . .	25
Installing on more than one management server . . . . .	26
Installing IBM Power CIM Provider . . . . .	27
Installing the IBM License Tool and activating the premium features . . . . .	28
Upgrading to IBM Hardware Management Pack Version 5.5. . . . .	28
Upgrading more than one management server . . . . .	28
Uninstalling the IBM Hardware Management Pack, version 5.5. . . . .	28
Deleting the IBM Hardware Management Packs . . . . .	29
Removing the IBM Power CIM Provider. . . . .	30
Uninstalling the software package. . . . .	30
Downgrading to a previous version . . . . .	31
Reinstalling IBM Hardware Management Pack, version 5.5. . . . .	31
Configuring BladeCenter SNMP settings. . . . .	31
Discovering a BladeCenter in Operations Manager 2007 . . . . .	34
Discovering a BladeCenter in Operations Manager 2012 . . . . .	37
Removing a discovered BladeCenter chassis . . . . .	44
Discovering an IBM Flex System Chassis enabled for SNMP . . . . .	45
Enabling SNMPv1 Agent . . . . .	48
Enabling SNMPv3 Agent . . . . .	49
Discovering an IBM Flex System in Operations Manager 2007 . . . . .	50
Discovering an IBM Flex System in Operations Manager 2012 . . . . .	51
Removing a discovered IBM Flex System chassis . . . . .	52

<b>Chapter 5. Working with the IBM Hardware Management Pack</b> . . . . .	<b>53</b>
Monitoring through the Operations Manager Console. . . . .	53
Adding an IBM system that will be managed by the Operations Manager . . . . .	61
Optional steps before starting this task . . . . .	61
How to check software dependencies on the remote computer . . . . .	61

Using the Discovery Wizard to add an IBM system	63
Viewing inventory . . . . .	72
Monitoring the health of systems, hardware components, and other targets . . . . .	72
Viewing alerts . . . . .	74
Locating and viewing hardware errors . . . . .	75
Using Health Explorer to identify and resolve problems . . . . .	75
Using knowledge pages to resolve problems . . . . .	77
Using premium features . . . . .	80
Remote power on and off of BladeCenter x86/x64 Blade servers . . . . .	81
Remote shut down of an operating system . . . . .	81
Remote Power On using the server name . . . . .	84
Setting the power threshold . . . . .	86
Enabling and setting power capping . . . . .	91
Setting the Predictive Failure Alert (PFA) Policy . . . . .	97
Viewing the power data for client System X servers . . . . .	99
Discovering the Flex System OOB-IB Reflection . . . . .	100
Using Flex system remote power on and off . . . . .	102
Launching the IBM Flex System Chassis Web Console . . . . .	106
Discovering an IBM Flex System Chassis FSM . . . . .	109
Launching the IBM Flex System Chassis FSM Web Console. . . . .	111

<b>Chapter 6. Working with Hardware Failure Management . . . . .</b>	<b>117</b>
Enabling Hardware Failure Management using the Operations Manager Console . . . . .	117
IMM discovery and authentication . . . . .	117

Using the power management feature for Hardware Failure Management . . . . .	121
--	-----

**Appendix A. Best practices . . . . . 123**

Best practice: Determining the cause of an error . . . . .	123
Best practice: Rediscovering all BladeCenters . . . . .	126
Best practice: Rediscovering a renamed server . . . . .	127

**Appendix B. Troubleshooting . . . . . 129**

Troubleshooting errors returned from the IBM Power CIM Provider . . . . .	129
Troubleshooting the installation of the IBM Power CIM Provider . . . . .	129
Verifying an IBM Power CIM installation finished successfully . . . . .	129
How to fix a failed IBM Power CIM Provider installation . . . . .	130
How to remove an IBM Chassis in Network Devices Pending Management on Windows server 2012 . . . . .	132
How to fix a failed task of opening an IBM System Web Console on an SCOM Console using Windows Server 2012 . . . . .	132

**Appendix C. Accessibility features 135**

**Notices . . . . . 137**

Trademarks . . . . .	138
Important notes . . . . .	138

**Index . . . . . 141**

---

## Figures

1. Software License Agreement . . . . .	21	48. Example of a critical error showing up in a managed system . . . . .	76
2. Trial Version . . . . .	22	49. Example of hardware components causing a system to be in error . . . . .	76
3. Destinations folder . . . . .	23	50. Example of hardware components causing a system to be in error . . . . .	78
4. SCVMM Server FQDN Configuration . . . . .	23	51. Example of a knowledge page that describes an error event. . . . .	79
5. Ready to Repair Program . . . . .	24	52. Example of one knowledge page linking to another . . . . .	79
6. Default SNMP ports . . . . .	32	53. Example of Alert Properties . . . . .	80
7. Enabling alerts using SNMP . . . . .	33	54. Operations Manager Console premium feature is enabled example . . . . .	81
8. Remote Alert Recipient. . . . .	33	55. Task Status for Shutdown Operating System on this Blade . . . . .	82
9. Monitored alerts . . . . .	34	56. Task status indicating the shutdown task has been sent to this Blade . . . . .	83
10. Discovery Wizard . . . . .	35	57. Example of a Task Output message . . . . .	84
11. Discovery Method . . . . .	36	58. Example of Blade Server Power On task . . . . .	85
12. Select Objects to Manage . . . . .	37	59. Task Output status for Power On task . . . . .	85
13. Discovery types . . . . .	38	60. Task Output when premium feature is not enabled . . . . .	86
14. General Properties page . . . . .	39	61. Example of Set/Unset Power Threshold task . . . . .	87
15. Introduction . . . . .	40	62. Target and task parameters of Set/Unset Power Threshold task . . . . .	88
16. Devices . . . . .	41	63. Override the task parameters of Set/Unset Power Threshold task . . . . .	89
17. Creating the discovery warning. . . . .	42	64. New values of the task parameters of Set/Unset Power Threshold task . . . . .	90
18. Discovery Wizard Completion . . . . .	43	65. Task Status indicating the Set/Unset Power Threshold task has been sent to the target server . . . . .	91
19. Discovery Rules . . . . .	44	66. Example of Set Power Capping task . . . . .	92
20. Default SNMP ports . . . . .	45	67. Target and task parameters of the Set Power Capping task . . . . .	93
21. Setting default SNMP ports . . . . .	46	68. Override the Task Parameters of Set Power Capping task . . . . .	94
22. Selecting Event Recipients. . . . .	46	69. New values of the Task Parameters of Set Power Capping task . . . . .	95
23. Create Event Recipients . . . . .	46	70. Task Status indicating the Set Power Capping task has been sent to the target server. . . . .	96
24. Creating an SNMP Recipient. . . . .	47	71. Set Predictive Failure Alerts Policy task example. . . . .	97
25. Event Recipient Global Settings . . . . .	47	72. PFA Policy Configuration window . . . . .	98
26. Simple Network Management Protocol (SNMP). . . . .	48	73. IBM System x Power Data Chart . . . . .	99
27. Security Policy setting . . . . .	49	74. Check IBM Flex System Chassis . . . . .	100
28. Account credentials for creating a new user for SNMPv3 devices . . . . .	50	75. Checking IBM Flex System Chassis Compute Nodes . . . . .	101
29. Monitoring pane . . . . .	54	76. Example of an IBM Licensed System Group . . . . .	101
30. Windows Computers on IBM System x or x86/x64 Blade Server view . . . . .	55	77. Example of an IBM x86/64 Flex OOB-IB Reflection Group . . . . .	102
31. IBM BladeCenter(s) and Modules folder view . . . . .	56	78. Example of remote power options for IBM Flex System Chassis Compute Nodes . . . . .	103
32. IBM Flex System Chassis folder view . . . . .	57	79. Window for remote power on task for Flex systems . . . . .	104
33. IBM Flex System Chassis Modules . . . . .	58	80. Task status for remote power on . . . . .	105
34. IBM BladeCenter Modules . . . . .	59		
35. Dashboard view . . . . .	60		
36. Hardware Management Software Configuration Advisor for IBM Systems program . . . . .	62		
37. PowerShell example of net view . . . . .	62		
38. Using the context menu to select the Discovery Wizard . . . . .	63		
39. Using the context menu to select the Discovery Wizard (SP1) . . . . .	64		
40. Computer and Device Manager Introduction . . . . .	65		
41. Selecting Auto or Advanced Discovery Method . . . . .	66		
42. Discovery Method . . . . .	67		
43. Discovery Method with sample information . . . . .	68		
44. Select Objects to Manage . . . . .	69		
45. Computer and Device Management Wizard Summary . . . . .	70		
46. Agent Management Task Status. . . . .	71		
47. Active Alerts example . . . . .	73		

81. Task Status indicating power on failed because no license is installed . . . . .	106	93. Example of launching an FSM Web Console from the SCOM console . . . . .	114
82. Example of launching the IBM Flex System Chassis Management Web Console . . . . .	107	94. FSM Web Console log in . . . . .	115
83. Certificate error when opening IBM Flex System Chassis Management Web Console. . . . .	107	95. IMM Discover Console . . . . .	118
84. Loading CMM Web Console . . . . .	108	96. IMM Discovery . . . . .	119
85. CMM Web Console . . . . .	108	97. Integrated Management Module . . . . .	120
86. CMM Console . . . . .	109	98. IMM Authentication . . . . .	120
87. Example of an IBM Flex System Chassis FSM . . . . .	110	99. Power Capping Management . . . . .	121
88. Refreshing the Chassis's Module . . . . .	110	100. Example of selecting a system with a critical state . . . . .	123
89. Example of setting the FSM IP address from the SCOM console . . . . .	111	101. Detailed view of a power module in critical state . . . . .	124
90. Run Task - Set FSM IP Address window . . . . .	112	102. System x Windows Management Instrumentation (WMI) event . . . . .	125
91. Example of overriding FSM IP address . . . . .	113	103. Example of the State Change Events tab detail information . . . . .	126
92. Task Status of Setting FSM IP Address indicating the task successfully completed . . . . .	114	104. Deleting a renamed server . . . . .	127



---

## Tables

1. Supported servers . . . . .	5	9. Requirements of ServeRAID-8x/7x/6x . . . . .	15
2. Supported IBM BladeCenter chassis . . . . .	7	10. IBM Hardware Management Pack versions required for Microsoft System Center Operations Manager 2007 . . . . .	18
3. Supported IBM Flex System chassis . . . . .	7	11. IBM Hardware Management Pack versions required for Microsoft System Center Operations Manager 2012 . . . . .	18
4. Agentless support matrix . . . . .	8	12. SNMP settings . . . . .	32
5. IBM Systems Director Agent . . . . .	12		
6. Supported configurations of IBM Systems Director Agent . . . . .	12		
7. Requirements for ServeRAID-MR or MegaRAID. . . . .	14		
8. Requirements for ServeRAID-BR/IR or Integrated RAID . . . . .	14		



---

## About this publication

This book provides instructions for installing the IBM® Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 into Microsoft System Center Operations Manager and using its integrated features to manage systems in your environment.

---

## Conventions and terminology

Paragraphs that start with a bold **Note**, **Important**, or **Attention** are notices with specific meanings that highlight key information.

**Note:** These notices provide important tips, guidance, or advice.

**Important:** These notices provide information or advice that might help you avoid inconvenient or difficult situations.

**Attention:** These notices indicate possible damage to programs, devices, or data. An attention notice appears before the instruction or situation in which damage can occur.



---

## Information resources

You can find additional information about the IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 in the product documentation and on the World Wide Web.

---

## PDF files

You have the option to view or print documentation that is available in Portable Document Format (PDF).

### Downloading Adobe Acrobat Reader

You need Adobe Acrobat Reader to view or print the PDF files. You can download a copy from the Adobe Reader Web site.

### Viewing and printing PDF files

You can view or print any of the PDF files located on the web. The most current version of each document is available on the product download page. Click the following link to locate the individual product pages for each publication: IBM System x Integration Offerings for Microsoft Systems Management Solutions.

---

## World Wide Web resources

The following web sites provide resources for understanding, using, and troubleshooting IBM System x, IBM Flex Systems, BladeCenter servers, and systems-management tools.

### IBM System x Integration Offerings for Microsoft Systems Management Solutions site

Locate the latest downloads for the IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5.

IBM System x Integration Offerings for Microsoft Systems Management Solutions

### IBM Systems Technical support site

Locate support for IBM hardware and systems-management software.

IBM Support Portal

## **IBM Systems Director: Download Software Registration site**

Download IBM systems-management software, including IBM Systems Director.

IBM Systems Director: Downloads

## **IBM Systems Management for System x site**

Provides an overview of IBM systems management using IBM Director Agent and IBM Director Core Services.

IBM systems management solutions for System x

## **IBM ServerProven sites**

Obtain information about hardware compatibility with IBM System x, xSeries servers, and IBM BladeCenter®, and IBM IntelliStation® hardware.

- System x and xSeries ServerProven: IBM ServerProven Compatibility for hardware, applications, and middleware
- BladeCenter ServerProven: IBM ServerProven Compatibility for BladeCenter products

## **Microsoft System Center Operations Manager site**

Obtain information about Microsoft System Center Operations Manager and how to monitor your IBM systems across large organizations using IBM and Microsoft applications.

Technet: Systems Center Technical Resources

---

# Chapter 1. IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5

The IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 enables customers to use the enhanced features of Microsoft System Center Operations Manager for managing the health state of IBM System x servers, Blades, IBM BladeCenter Chassis, Compute Nodes, and IBM Flex System® Chassis.

The IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 has a new feature, Hardware Failure Management, for enhancing the Reliability, Availability, Serviceability (RAS) capability of IBM hardware server products. In short, this feature automatically migrates virtual machines from a server host where hardware failures are detected to other server hosts.

---

## Key features

The key features of the IBM Hardware Management Pack are:

- Rich monitoring of system health using SNMP protocol for: IBM BladeCenter Chassis, IBM Flex System Chassis and modules
- Extensive monitoring of the hardware component health for IBM System x servers, BladeCenter x86/x64 blades, and Flex System x86/x64 compute nodes running Windows
- Comprehensive monitoring of the software stack health for managing IBM hardware
- Easy determination of overall system health by the aggregation of hardware health monitors
- Automatic migration of virtual machines from a server host, where hardware failures are detected, to other server hosts

---

## Premium features

IBM Upward Integration for Microsoft System Center has several premium features which require an activation license.

The following additional features are fee-based and require the purchase of an activation license on a per managed endpoint basis. Activation licenses can be purchased by contacting either your IBM representative or an IBM Business Partner. These features offer the ability to:

- Establish Out-of-band - In-band (OOB-IB) communication using reflection to synchronize the information obtained out-of-band (using SNMP) and in-band (using OS).
- Launch a Flex System Chassis CMM Web Console from the Operations Manager Console.
- Discover a Flex System Manager (FSM) device and launch an FSM Console in the Operations Manager Console.
- Monitor Flex System Chassis and Chassis modules using both SNMPv1 and SNMPv3. This feature requires the installation of the 4.0 license tool; the activation version is 255.0.

- Launch a Windows IMM Web Console server from the Operations Manager console. This feature requires the installation of the 4.0 license tool; the activation version is 255.0.
- Utilize Active Power Management and Monitoring on uEFI and IMM System x servers and blades running Windows 2008 and Windows 2008 R2 with IBM Director Platform Agent v6.2.1 or later. You can monitor and manage the overall system power usage and generate alerts when power consumption rises above predefined consumption thresholds.
- Customize and set power consumption thresholds for power monitoring alerts.
- Set and enable power capping thresholds to manage maximum power consumption wattage.
- Monitor the power data of client System x systems by viewing the System x Power Data Chart.
- Reflect the health of the BladeCenter x86/x64 modules to the BladeCenter x86/x64 blade servers affected by those modules. BladeCenter and Blade hardware health correlation and event propagation provides BladeCenter specific hardware health condition monitoring under the Windows health explorer view.
- Enable the Hardware Management Software Configuration Advisor for IBM Systems (SW Configuration Advisor) program, which analyzes software dependencies of the IBM Hardware Management Pack on a managed Microsoft Windows system. The program is run from the Operations Manager management server. SW Configuration Advisor detects the presence of the IBM Hardware Management Pack software dependencies, and makes appropriate configuration recommendations.
- Provides the ability to remotely power on and off blade servers using the Operations Manager console.
- Discover the Integrated Management Module (IMM), and correlate it with the host.
- Set the predictive failure alert (PFA) policy to IMM for Brickman base Systems.

**Note:** All of the features listed above are available when the licensed feature level is at least 3.0, unless version 5.0 is noted for a particular licensed feature level.

---

## Trial license support

A trial license is automatically activated if a product license is not activated, when installing this product for the first time. After the trial license has been activated, the trial period is 90 days. During the trial period, the premium features are enabled.

**Important:** Before allowing the trial license to become activated, you need to verify that your system time is correct.

After the trial license expires, the premium features are disabled unless a product license is activated. You can obtain a product license from: IBM Upward Integration for MSSC.

To view the license information for each managed server, click **Monitoring IBM Hardware IBM Licensed System Group**. The license information for each IBM server is displayed in the **IBM HW Management Licensed System** column.



---

## Chapter 2. Technical overview

The topics in this section describe how the Microsoft System Center Operations Manager monitors the health of a management target, performs hardware failure management, authors management packs, and performs administrative operations.

A management target in the Microsoft System Center Operations Manager can be a computer system, an operating system instance, an application, a network adapter, or a subcomponent within a management target. The IBM Hardware Management Pack provides management innovation for its IBM management targets. This scope of management classifies the Operations Manager as a systems management software tool.

Upon discovering a Windows system, the Microsoft System Center Operations Manager management server pushes the Microsoft System Center Operations Manager agent onto the system, along with scripts inside the IBM Hardware Management Pack that provide policies for monitoring health and collecting events.

With the Microsoft System Center Operations Manager, you can create custom groups of objects to manage a holistic health aggregation based on your business needs. You can define different monitoring and aggregation rules for different groups.

For example, an application hosting provider might have a per-client holistic health view of all of the hardware, operating systems, applications, and other objects involved with the client. The hosting provider might also have a per-application view or have both views available at the same time.

Microsoft System Center Operations Manager maintains operations databases for tracking all events that are reported. Expert analysis of the operations databases can show deep cause and effect relationships in the historical data that can reveal the root cause of a sophisticated problem.

The Operations Manager reports cooling fan availability based on the fan presence sensor reading and the fan performance according to the fan tachometer reading. The IBM Hardware Management Pack establishes relationships for hosting and aggregating, and also establishes health dependency among the IBM management targets. The Operations Manager provides health roll-ups and drill-downs to give you a holistic view of objects, and to allow you to quickly identify a specific problem.

---

## How the IBM Hardware Management Pack supports IBM systems

With IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 you can use the enhanced features of Microsoft System Center Operations Manager to communicate with Flex System Management modules, BladeCenter Management modules, System x, and x86/x64 Blade servers installed with IBM Director Core Services or Platform Agent to discover and monitor the health of:

- IBM BladeCenter Chassis and chassis components
- IBM Flex System Chassis and chassis components
- IBM System x systems and BladeCenter blade server systems

Because the IBM Hardware Management Pack communicates with the IBM Flex System Chassis, IBM BladeCenter Chassis and components, and individual IBM System x, Flex Chassis x86/x64 Compute Node, and BladeCenter x86/x64 blade servers, you can use Microsoft System Center Operations Manager to monitor all Flex chassis, BladeCenter chassis, and Windows-based IBM servers holistically.

The IBM Hardware Management Pack communicates with Flex System and BladeCenter chassis and chassis components through the management module using Simple Network Management Protocol (SNMP) over a LAN.

The IBM Hardware Management Pack communicates with individual servers, including BladeCenter Blade servers, which are running a Windows operating system and that have a supported version of IBM Director Core Services or Platform Agent installed.

---

## Management concepts

This topic describes management concepts as they apply to a BladeCenter being managed by the Microsoft System Center Operations Manager.

After Microsoft System Center Operations Manager selects a server to manage, it pushes its Operations Manager Agent onto the managed system with the IBM Hardware Management Pack, if the target is an IBM System x or BladeCenter x86/x64 Blade server. The Operations Manager Agent and the IBM Hardware Management Pack communicate with the IBM Director Agent and other software for hardware management on the system and across the network to the Operations Manager server.

**Note:** These management functions are supported on the IBM BladeCenter chassis, IBM Flex System chassis, and on IBM System x and x86/x64 Blade servers and compute nodes running Windows operating system. These functions are not supported on System i<sup>®</sup>, System p, and System z systems.

---

## Chapter 3. Supported configurations

IBM Hardware Management Pack has specific requirements for hardware and software. The topics in this section provide detailed information about configurations, hardware, and software supported by this release of the IBM Hardware Management Pack.

---

### Supported systems

The IBM Hardware Management Pack supports the following systems:

#### Supported IBM servers

IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 supports the following servers:

*Table 1. Supported servers*

Server Product Name	Machine Type
IBM BladeCenter HS12	8014, 8028
IBM BladeCenter HS21	8853
IBM BladeCenter HS22	7870*, 1911
IBM BladeCenter HS22V	7871*
IBM BladeCenter HS23	7875*
IBM BladeCenter HS23E	8038*, 8039*
IBM BladeCenter HX5	7872*, 7873*
IBM BladeCenter LS21	7971
IBM BladeCenter LS22	7901
IBM BladeCenter LS41	7972
IBM BladeCenter LS42	7902
IBM Flex System x220 Compute Node	7906, 2585
IBM Flex System x222 Compute Node	7916
IBM Flex System x240 Compute Node	8737, 7863, 8956
IBM Flex System x440 Compute Node	7917
IBM Flex System x880 Compute Node	4259, 7903
IBM NeXtScale Node	5455, 5456
IBM System x3100 M5	5457
IBM System x3100 M4	2582, 2586
IBM System x3200 M2	4367, 4368
IBM System x3200 M3	7327*, 7328*
IBM System x3250 M2	4190, 4191, 4194
IBM System x3250 M3	4251*, 4252*, 4261
IBM System x3250 M4	2583, 2587
IBMSystem x3250 M5	5458
IBM System x3300 M4	7382

Table 1. Supported servers (continued)

Server Product Name	Machine Type
IBM System x3350	4192, 4193
IBM System x3400 M2	7836*, 7837*
IBM System x3400 M3	7378*, 7379*
IBM System x3450	7948, 7949, 4197
IBM System x3455	7940, 7941
IBM System x3500 M2	7839*
IBM System x3500 M3	4254, 7944*
IBM System x3500 M4	7383*
IBM System x3530 M4	7160
IBM System x3550	7978
IBM System x3550 M2	7946*
IBM System x3550 M3	4254, 7944*
IBM System x3550 M4	7914*
IBM System x3620 M3	7376*
IBM System x3630 M3	7377*
IBM System x3630 M4	7158*
IBM System x3650	7979
IBM System x3650 M2	7947*
IBM System x3650 M3	4255, 7945*
IBM System x3650 M4	7915*
IBM System x3650 M4 BD	5466
IBM System x3650 M4 HD	5460
IBM System x3650 T	7980, 8837
IBM System x3655	7985
IBM System x3690 X5	7147, 7148*, 7149*, 7192
IBM System x3750 M4	8752
IBM System x3755	7163, 8877
IBM System x3755 M3	7164
IBM System x3850 M2/x3950 M2	7141, 7144, 7233, 7234
IBM System x3850 X5/x3950 X5	7143, 7145*, 7146*, 7191
IBM System x3850 X6/x3950 X6	3837, 3839
IBM System x3850 MAX5/x3950 MAX5	7145*, 7146*
IBM System x iDataPlex® dx360 M2	6380*, 7323*, 7321*
IBM System x iDataPlex dx360 M3	6391
IBM System x iDataPlex Direct Water Cooled dx360 M4	7918*, 7919*
IBM System x iDataPlex dx360 M4	7912*, 7913*

**Note:** Fee-based Power Monitoring support is available for the systems denoted with an "\*" if the system has the latest firmware. Power management requires the system is running Windows 2008 or Windows 2008 R2 and the IBM Director Agent

v6.2.1 or later. For more information, see “Supported configurations of managed systems with Power Monitoring” on page 15.

For a description of the compatibility of a specific system with Windows and other hardware components, see “World Wide Web resources” on page xi and the respective ServerProven<sup>®</sup> page for that system.

## Supported IBM BladeCenter chassis

IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 supports the following IBM BladeCenter chassis:

*Table 2. Supported IBM BladeCenter chassis*

Machine Name	Machine Type
IBM BladeCenter	7967
IBM BladeCenter E	8677
IBM BladeCenter H	8852, 7989
IBM BladeCenter S	8886, 7779
IBM BladeCenter T	8720, 8730
IBM BladeCenter HT	8740, 8750

## Supported IBM Flex System chassis

IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 supports the following IBM Flex System chassis:

*Table 3. Supported IBM Flex System chassis*

Machine Name	Machine Type
IBM Flex System Chassis	7893, 8721, 8724

## Agentless support

IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 supports the collection of information for the following hardware options.

Table 4. Agentless support matrix

Agentless hardware support list		Flex System x 240	Flex System x 440	Flex System x220	Flex System x222	Flex System x880 X6	System x3850 X6/x3960 X6
LSI	LSI2004 RAID	-	-	-	-	✓	-
	ServeRAID M5120 SAS/SATA Controller (81Y4478)	-	-	-	-	-	✓
	ServeRAID M5115 SAS/SATA Controller (90Y4390)	✓	✓	✓	-	✓	-
	ServeRAID M5210 SAS/SATA Controller (46C9110)	-	-	-	-	-	✓
Qlogic	IBM Flex System FC3172 2-port 8Gb FC Adapter (69Y1938)	✓	✓	✓	-	✓	-
	IBM Flex System FC 5172 2-port 16Gb FC Adapter (69Y1942)	✓	✓	✓	-	✓	-
Emulex	IBM Flex System CN4054R 10Gb Virtual Fabric Adapter (00Y3306)	✓	✓	✓	-	✓	-
	IBM Flex System FC5052 2-port 16Gb FC Adapter (95Y2386)	✓	✓	✓	-	✓	-
	IBM Flex System FC5054 4-port 16Gb FC Adapter (95Y2391)	✓	✓	✓	-	✓	-
	IBM Flex System FC3052 2-port 8Gb FC Adapter (95Y2375)	✓	✓	✓	-	✓	-
	Emulex BE3 Enet	✓	-	-	-	-	-
	IBM Virtual Fabric Advanced Software Upgrade (90Y9310)	-	✓	-	✓	-	-

Table 4. Agentless support matrix (continued)

Agentless hardware support list		Flex System x 240	Flex System x 440	Flex System x220	Flex System x222	Flex System x880 X6	System x3850 X6/x3960 X6
Mellanox	IBM Flex System IB6132 2-port FDR Infiniband Adapter (90Y3454)	✓	✓	✓	-	✓	-
	IBM Flex System EN4132 2-port 10Gb Ethernet Adapter (90Y3466)	✓	✓	✓	-	✓	-
	IBM Flex System IB6132 Infiniband Adapter	-	-	-	✓	-	-
	IBM Flex System EN6132 2-port 40Gb Ethernet Adapter (90Y3482)	✓	✓	✓	-	✓	-
Broadcom	IBM Flex System EN2024 4-port 1Gb Ethernet Adapter (49Y7900)	✓	✓	✓	-	✓	-
	IBM Flex System CN4022 2-port 10Gb Converged Adapter (88Y5920)	✓	✓	-	-	✓	-
	Kestrel LOM	-	-	✓	-	-	-
Brocade	IBM Flex System FC5022 2-port 16Gb FC Adapter (88Y6370)	✓	✓	✓	-	✓	-
	IBM Flex System FC5024D 4-port 16Gb FC Adapter (95Y2379)	-	-	-	✓	-	-

---

## Supported configurations of management servers

Use the topics in this section to determine whether a system can be supported by the IBM Hardware Management Pack as a management server. A management server is supported if it meets the requirements for Systems Center Operations Manager and is on a supported hardware configuration.

### Supported versions of Microsoft System Center Operations Manager for management servers

The following versions of Microsoft System Center Operations Manager for management servers are supported:

- Microsoft System Center Operations Manager 2012
- Microsoft System Center Operations Manager 2012 R2
- Microsoft System Center Operations Manager 2012 SP1
- Microsoft System Center Operations Manager 2007
- Microsoft System Center Operations Manager 2007 R2

### Prerequisites for Hardware Failure Management

- Microsoft System Center Operations Manager (SCOM) and System Center Virtual Machine Manager (SCVMM) are installed
- Managed nodes (IBM hardware servers) are in clusters and managed by SCVMM and SCOM
- Verification that the Integrated Management Module (IMM) for the IBM hardware servers is correctly set, including the IP address, CIM, SLP, and user accounts

### Supported operating systems for management servers

This topic provides a list of supported operating systems for management servers and links to additional information:

#### Microsoft System Center Operations Manager 2012

System Requirements: System Center 2012 - Operations Manager

#### Microsoft System Center Operations Manager 2012 R2

System Requirements: System Center 2012 R2 Operations Manager

#### Microsoft System Center Operations Manager 2012 SP1

System Requirements: System Center 2012 SP1 - Operations Manager

#### Microsoft System Center Operations Manager 2007 SP1

Operations Manager 2007 SP1 Supported Configurations for the supported operating systems: Refer to the "Management server or root management server" row.

#### Microsoft System Center Operations Manager 2007 R2

Operations Manager 2007 R2 Supported Configurations for the supported operating systems: Refer to the "Management server or root management server" row.

**Note:** Operations Manager 2007 SP1 is supported on Windows Server 2008 and Windows Server 2008 SP1/R2, but requires that you apply a set of hot fixes.

For more information, see:

- Support for running Microsoft System Center Operations Manager Service Pack 1 and System Center Essentials 2007 Service Pack 1 on a Windows Server 2008-based computer



- Microsoft System Center Operations Manager 2007 SP1 Update Rollup.

### **Additional configuration requirements for management servers**

All Operations Manager management servers within the same management group, require the same version of the IBM Hardware Management Pack is installed. Therefore, a mixed version of management packs is not supported.

- Management servers managing IBM BladeCenters require one of the following versions of the IBM Hardware Management Pack is installed and imported to the Operations Manager:
  - IBM.HardwareMgmtPack.BladeCenter.mp
  - IBM.HardwareMgmtPack.BladeCenter.v2.mp
- Management servers managing IBM Flex System chassis require one of the following versions of the IBM Hardware Management Pack is installed and imported to the Operations Manager:
  - IBM.HardwareMgmtPack.FlexSystem.mp
  - IBM.HardwareMgmtPack.FlexSystem.v2.mp

---

## **Supported configurations and requirements for a managed system**

The topics in section describe supported configurations and requirements for a managed system.

A properly configured managed system has the following requirements:

- It is managed in an Operations Manager management group by a management server with a supported configuration.
- It is installed on a supported server. For more information, see “Supported systems” on page 5.
- It is running a supported version of Windows operating system.
- It is running the required software for hardware management.

## **Supported operating systems for managed systems**

This topic provides a list of supported operating systems for managed systems and links to additional information.

### **Microsoft System Center Operations Manager 2012**

System Requirements: System Center 2012 - Operations Manager

### **Microsoft System Center Operations Manager 2012 R2 System Requirements: System Center 2012 R2 Operations Manager**

### **Microsoft System Center Operations Manager 2012 SP1**

System Requirements: System Center 2012 SP1 - Operations Manager

### **Microsoft System Center Operations Manager 2007 R2**

Operations Manager 2007 R2 Supported Configurations: Refer to the "Agent" row.

### **Microsoft System Center Operations Manager 2007 SP1**

Operations Manager 2007 SP1 Supported Configurations: Refer to the "Agent" row.

## Supported versions of IBM Systems Director Agent

A managed Windows system requires a supported version of IBM Systems Director Agent is installed and running.

The following table provides a list of IBM Systems Director Agent versions and indicates whether the version is supported for a managed Windows system.

*Table 5. IBM Systems Director Agent*

IBM Systems Director Agent version	Supported by IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5	Notes
6.3, 6.3.1, 6.3.2, 6.3.3	Supported	Platform Agent and Common Agent are supported.
6.2.0, 6.2.1	Supported	Platform Agent and Common Agent are supported.
6.1.1, 6.1.2	Supported	Platform Agent and Common Agent are supported.
5.20, 5.20.1, 5.20.2, 5.20.3x	Supported	IBM Director Core Services (also called Level-1 Agent) or Level-2 Agent

## Supported configurations of IBM Systems Director Agent

The following table provides a list of information resources for the hardware and software supported by each version of IBM Systems Director Agent.

*Table 6. Supported configurations of IBM Systems Director Agent*

IBM Systems Director Agent version	Supported hardware and software resources
6.3, 6.3.1, 6.3.2, 6.3.3	To view the most current IBM systems and products, and operating systems for v6.3.x, refer to: IBM Systems Director V6.3.x Information Center and select the applicable 6.3.x version.
6.2.0, 6.2.1	<ul style="list-style-type: none"> <li>To view a list of supported IBM systems and products for v6.2.x, refer to: Supported IBM systems and products for v6.2.x.</li> <li>To view a list of supported Windows operating systems for v6.2.x, refer to: Supported operating systems for v6.2.x.</li> </ul>
6.1.2	<ul style="list-style-type: none"> <li>To view a list of supported IBM systems and products for v6.1.x, refer to: Supported IBM systems and products for v6.1.x.</li> <li>To view a list of supported Windows operating systems for v6.1.x, refer to: Operating systems supported by IBM Systems Director 6.1.2.</li> </ul>
5.20.x	<ul style="list-style-type: none"> <li>To view a list of supported systems and products for v5.20, refer to: Supported Hardware for IBM Director V5.20.</li> <li>To view a list of supported Windows operating systems for v5.20, refer to: Operating systems supported by IBM Director 5.20.</li> </ul>

## Supported configurations of managed systems with BMC or IPMI

A managed Windows system, with a Baseboard Management Controller (BMC) or an Intelligent Platform Management Interface (IPMI), requires a supported version of the IPMI driver stack is installed and running.

- **For Windows Server 2000 or Windows Server 2003**, both the OSA IPMI device driver and the IBM Mapping Layer for OSA IPMI driver are required. The OSA IPMI device driver for Windows is available at: [OSA IPMI device driver support and downloads](#).
- **For Windows Server 2003 R2**, the IPMI driver must be installed and running. The Microsoft IPMI driver is not installed by default.
- **For all versions of Windows Server 2008**, the Microsoft IPMI driver is required. The Microsoft IPMI driver is automatically installed on IBM servers that come with BMC or an IPMI. There is no need to install the IBM Mapping Layer for OSA IPMI driver with the Microsoft IPMI driver stack.

The IBM Mapping Layer for OSA IPMI for Windows is available at:

- [IBM Mapping Layer for OSA IPMI for x86 version](#)
- [IBM Mapping Layer for OSA IPMI for x64 version](#)

To acquire and apply the latest firmware for the Baseboard Management Controller or an Intelligent Platform Management Interface on a managed system, see the [IBM Support Portal](#).

## Supported configurations of managed systems with Remote Supervisor Adapter-II

A managed Windows system, with Remote Supervisor Adapter (RSA) II, requires the RSA-II daemon is installed and running.

The RSA-II daemon for Windows is available at:

- [IBM Remote Supervisor Adapter II for x86 version](#)
- [IBM Remote Supervisor Adapter II for x64 version](#)

For systems that come with a Baseboard Management Controller (BMC), which also have the RSA-II installed, the RSA-II daemon is optional, if a supported Intelligent Platform Management Interface (IPMI) driver stack is installed and running. However, the RSA-II daemon adds additional in-band system management functions to the functionality that is offered through the IPMI driver stack with a BMC.

IBM Systems Director Agent 6.x does not support systems that do not have a BMC but have only the RSA-II. Use IBM Systems Director Agent 5.20.3x with the RSA-II daemon for these systems.

To acquire and apply the latest firmware for RSA-II for a managed system, see the [IBM Support Portal.RSA-II](#).

## Supported configurations of managed systems with ServeRAID-MR or MegaRAID

This topic describes the supported configurations of managed systems with ServeRAID-MR or MegaRAID.

The following table lists the requirements of systems with ServeRAID-MR or MegaRAID.

*Table 7. Requirements for ServeRAID-MR or MegaRAID*

IBM Systems Director Agent	Additional software needed
6.3, 6.3.1, 6.3.2, 6.3.3	No additional software is needed. The IBM Power <sup>®</sup> CIM Provider is part of the Platform Agent.
6.2.0, 6.2.1	No additional software is needed. The IBM Power CIM Provider is part of the Platform Agent.
6.1.2	No additional software is needed. The IBM Power CIM Provider is part of the Platform Agent.
5.20.x	Download and install the LSI Mega RAID Provider for Windows from IBM Director 5.2 Downloads.

To download and install the latest firmware and device driver for the ServeRAID-MR or MegaRAID controller for a managed system, see the IBM Support Portal.

## Supported configurations of managed systems with ServeRAID-BR/IR or Integrated RAID

This topic describes the supported configurations of managed systems with ServeRAID-BR/IR or Integrated RAID.

The following table lists the requirements of systems with ServeRAID-BR/IR or Integrated RAID.

*Table 8. Requirements for ServeRAID-BR/IR or Integrated RAID*

IBM Systems Director Agent version	Additional software needed
6.3, 6.3.1, 6.3.2, 6.3.3	No additional software is needed. The IBM Power CIM Provider is part of the Platform Agent.
6.2.0, 6.2.1	No additional software is needed. The IBM Power CIM Provider is part of the Platform Agent.
6.1.2	No additional software is needed. The IBM Power CIM Provider is part of the Platform Agent.
5.20.x	Download and install the LSI Mega RAID Provider for Windows from IBM Director 5.2 Downloads.

To download and install the latest firmware and device driver for the ServeRAID-BR/IR or Integrated controller for a managed system, see the IBM Support Portal.

## Supported configurations of managed systems with ServeRAID versions 8x/7x/6x

This topic describes the supported configurations of managed systems with ServeRAID versions 8x/7x/6x. .

The following table lists the requirements of systems with ServeRAID controller versions 8x, 7x, and 6x:

*Table 9. Requirements of ServeRAID-8x/7x/6x*

IBM Systems Director Agent version	Additional software needed
6.3, 6.3.1, 6.3.2, 6.3.3	No additional software is needed. The IBM Power CIM Provider is part of the Platform Agent.
6.2.0, 6.2.1	No additional software is needed. The IBM Power CIM Provider is part of the Platform Agent.
6.1.2	Not supported.
5.20.x	Download and install the ServeRAID Manager 9.0 – Windows L1 Agent or ServeRAID Manager 9.0 – Windows L2 Agent from IBM Director 5.2 Downloads.

To download and install the latest firmware and device driver for the ServeRAID-8x/7x/6x controller for a managed system, see the IBM Support Portal.

## Supported configurations of managed systems with Power Monitoring

This topic describes supported configurations of managed systems with Power Monitoring.

The IBM Power CIM Provider has the following hardware and software requirements:

- The physical hardware requires the latest versions of IMM and uEFI. IMM supports power monitoring and/or power capping.  
For additional set up information see “Supported configurations of managed systems with BMC or IPMI” on page 13.
- IBM Systems Director Agent 6.2.1 or later
- The following Windows operating system versions:
  - Windows Server 2008
  - Windows Server 2008 SP1/R2
  - Windows Server 2008 SP1/R2 with Service Pack 1
  - Windows Server 2012



---

## Chapter 4. Installing the IBM Hardware Management Pack and other components

The topics in this section describe how to install, upgrade, uninstall, and reinstall the IBM Hardware Management Pack and other components.

The IBM Hardware Management Pack enhances the management of IBM systems in the Operations Manager along with the reliability, availability, and serviceability (RAS) of IBM hardware server products.

The IBM Hardware Management Pack discovers and monitors the health of the IBM BladeCenter chassis and chassis components and discovers the Integrated Management Modules (IMMs) and correlates them with the host.

---

### Overview of the installation process

The installation process starts by first installing a supported version of Microsoft System Center Operations Manager 2007 or 2012 on the management server.

For more information about the installation process, select one of the following options:

- Follow the instructions on the Deploying System Center 2012 - Operations Manager web page for installing Microsoft System Center Operations Manager 2012: Deploying System Center 2012 - Operations Manager.
- Follow the instructions on the Deploying System Center 2012 - Virtual Machine Manager web page for installing the Virtual Machine Manager: Deploying System Center 2012 - Virtual Machine Manager.

After Microsoft System Center Operations Manager and Virtual Machine Manager have been installed, the IBM Hardware Management Pack can be installed on the management server.

To add a Windows system that the Operations Manager will manage, which is on an IBM System x server or a IBM BladeCenter Blade server, use the Operations Manager Discovery Wizard.

When the IBM Hardware Management Pack installation is finished, the following Microsoft System Center Operations Manager functions are enhanced for IBM System x and BladeCenter x86 systems:

**Health explorer view:**

Examines the health state of IBM BladeCenter chassis and components, and individual servers at a component level in a hierarchical view of availability, configuration, performance, and security.

**Diagram view:**

Shows inner, organizational views of the IBM chassis, IBM System x, BladeCenter, and Compute Node x86/x64.

**Events view:**

Captures events that occur on specific or aggregate targets of IBM chassis, IBM System x, and System x x86/x64 systems.

**Active alerts view:**

Lists all alert notifications for specific or aggregate targets of IBM chassis, IBM System x, and IBM BladeCenter x86/x64 systems.

## Installation requirements for the IBM Hardware Management Pack

The following list outlines the installation requirements for installing the IBM Hardware Management Pack.

- You need to have administrative privileges for the system where you are installing the IBM Hardware Management Pack and also for the Operations Manager's management group where you importing the management packs.
- You install the IBM Hardware Management Pack on an IBM system that is running as a Microsoft System Center Operations Manager management server. The server can be the Root Management Server in the Operations Manager management group or a non-Root Management Server in the management group. See "Supported configurations of management servers" on page 10 for detailed requirements.
- If the IBM Hardware Management Pack is being installed on a server with Microsoft System Center Operations Manager 2007, you should install Microsoft .NET Framework 4.0 first.

The versions of the IBM Hardware Management Pack required for Microsoft System Center Operations Manager 2007 and 2012 are listed in the tables below. IBM Hardware Management Pack requires a minimum version as noted or a later, supported version.

*Table 10. IBM Hardware Management Pack versions required for Microsoft System Center Operations Manager 2007*

Management Pack name	Management Pack ID	Management Pack version
Health Library	System.Health.Library	6.0.5000.0
System Library	System.Library	6.0.5000.0
Performance Library	System.Performance.Library	6.0.5000.0
SNMP Library	System.Snmp.Library	6.0.6278.0
Data Warehouse Library	Microsoft.SystemCenter.Datawarehouse.Library	6.0.6278.0
System Center Core Library	Microsoft.SystemCenter.Library	6.0.5000.0
Network Device Library	Microsoft.SystemCenter.NetworkDevice.Library	6.0.6278.0
Windows Core Library	Microsoft.Windows.Library	6.0.5000.0

*Table 11. IBM Hardware Management Pack versions required for Microsoft System Center Operations Manager 2012*

Management Pack name	Management Pack ID	Management Pack version
Health Library	System.Health.Library	6.0.5000.0
System Library	System.Library	6.0.5000.0



Table 11. IBM Hardware Management Pack versions required for Microsoft System Center Operations Manager 2012 (continued)

Management Pack name	Management Pack ID	Management Pack version
Performance Library	System.Performance.Library	6.0.5000.0
SNMP Library	System.Snmp.Library	6.0.6278.0
Data Warehouse Library	Microsoft.SystemCenter.Datawarehouse.Library	6.0.6278.0
System Center Core Library	Microsoft.SystemCenter.Library	6.0.5000.0
Network Device Library	System.NetworkManagement.Library	7.0.8107.0
Windows Core Library	Microsoft.Windows.Library	6.0.5000.0

## Installing the IBM Hardware Management Pack

This topic provides some additional information that will assist you with the installation of the IBM Hardware Management Pack.

- For Microsoft System Center Operations Manager 2007, you can install the IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 on either a Root Management Server or a non-Root Management Server. A Root Management Server is the first management server in a management group, where you install the Operations Manager.
- For Microsoft System Center Operations Manager 2012, you can install the IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 on a non-Root Management Server.
- You must have a sufficient level of privilege and knowledge about the Root Management Server and non-Root Management Server before you can start the installation process.
- There is only one installation package for the IBM Hardware Management Pack for both the Windows 32-bit and 64-bit operating systems. To start the installation, follow the instructions for locating and launching the correct installation package in “Steps for installing the IBM Hardware Management Pack” on page 20.
- If you have an earlier version of the IBM Hardware Management Pack installed on a management server or the management packs have already been imported to the Operations Manager, see “Upgrading to IBM Hardware Management Pack Version 5.5” on page 28.

**Note:** You can install or uninstall of the IBM Hardware Management Pack by using the IBM Upward Integration for Microsoft System Center Integrated Installer. Refer to the IBM Upward Integration for Microsoft System Center Integrated Installer User's Guide for more information on how to perform this action.

## Steps for installing the IBM Hardware Management Pack

The following procedure describes how to install the IBM Hardware Management Pack.

### Before you begin

If you are running Microsoft System Center Operations Manager 2007 Service Pack 1 (SP1) on Windows Server 2008, install the service packs for both Windows Server 2008 and Microsoft System Center Operations Manager 2007 SP1 before proceeding with the IBM Hardware Management Pack installation.

For more information about how to install service packs, refer to: Support for running System Center Operations Manager 2007 Service Pack 1 and System Center Essentials 2007 Service Pack 1 on a Windows Server 2008-based computer.

### Procedure

1. On the IBM Hardware Management Pack for Microsoft System Center Operations Manager - IBM BladeCenter and System x web page in the File Details section, locate the file named **ibm\_sw\_hwmp\_x.x.x\_windows\_32-64.exe** and download IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5.
2. To start the installation process, double-click the downloaded installation executable file: `ibm_sw_hwmp_x.x.x_windows_32-64.exe`.  
Refer to Operations Manager 2007 R2 Quick Start Guide for more information on how to install Microsoft System Center Operations Manager 2007.  
Refer to Deploying System Center 2012 - Operations Manager for more information on how to install Microsoft System Center Operations Manager 2012.  
The Welcome to the InstallShield Wizard for IBM Hardware Management Pack for Microsoft Operations Manager v5.5 page opens.  
**Note:** If the installer cannot find Microsoft System Center Operations Manager on your system, the installation closes.
3. Click **Next**. The Software License Agreement page opens.

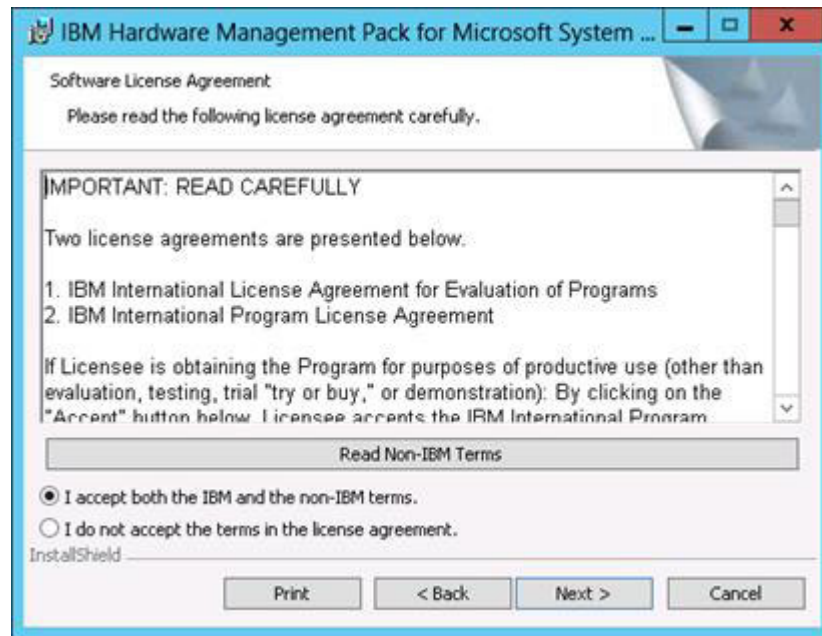


Figure 1. Software License Agreement

4. Read the software license agreements for IBM terms and click **Read Non-IBM Terms** to read the Non-IBM Terms. If you agree and accept both IBM and Non-IBM terms, select **I accept the IBM and the non-IBM term**; then click **Next**.

**Notes:**

- If this is the first installation of IBM Hardware Management Pack and no product license is activated, the Trial Version page opens. Complete step 5 for the Trial Version page.
- If a product license is activated, complete step 6.

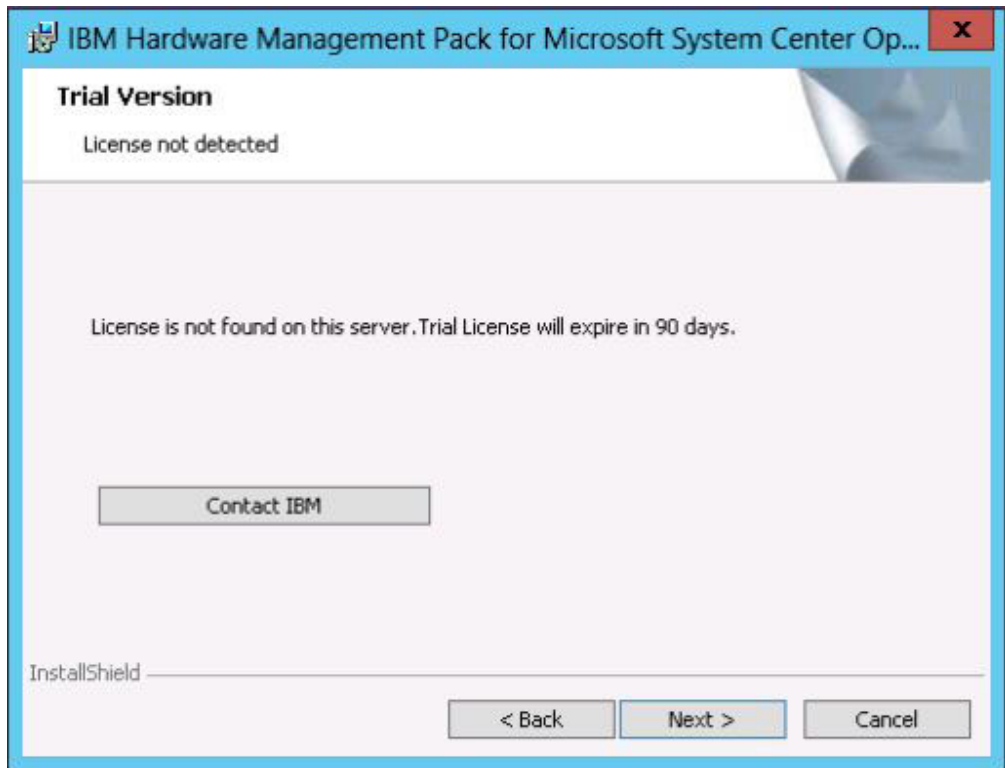


Figure 2. Trial Version

5. On the Trial Version page, select one of the following options:
  - **Contact IBM to obtain a valid product license** to obtain a product license.
  - **Next** to proceed to the Destination Folder page.
6. On the Destination Folder page, verify that the default target location is correct and click **Next**, or click **Change** to select the target folder for the installation software and then click **Next**.

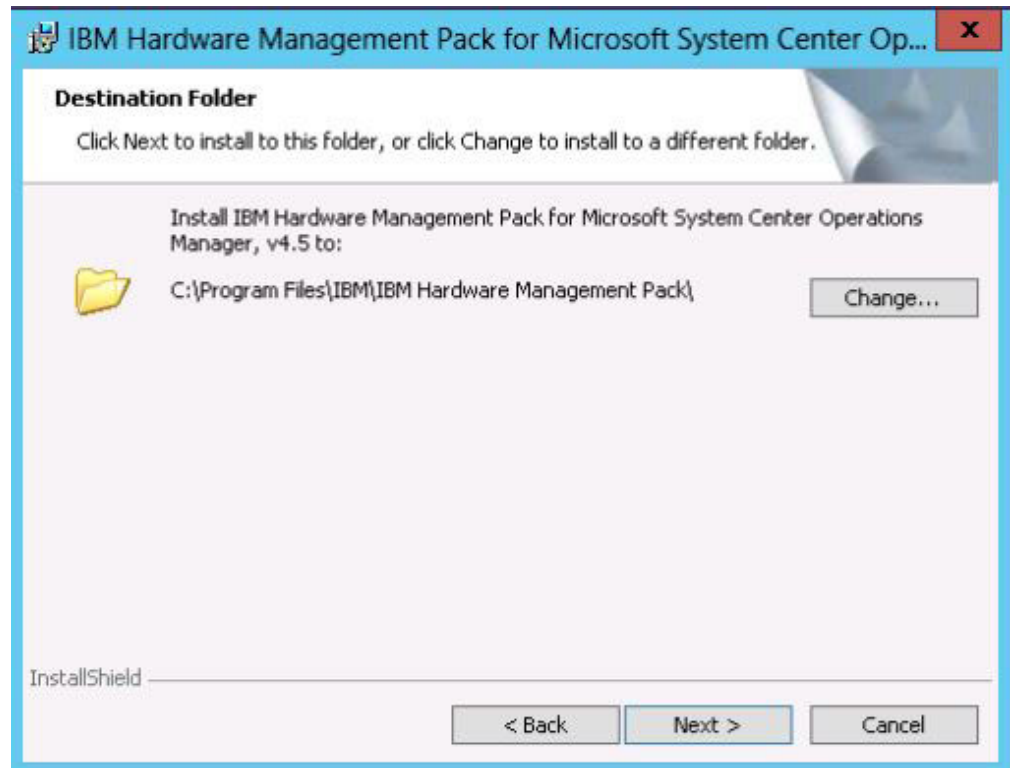


Figure 3. Destinations folder

7. On the FQDN Configuration page, complete one of the following steps:
  - Enter the name of the **SCVMM Server FQDN** to perform a VM migration and click **Next**, or
  - Click **Next** if you do not need to perform a VM migration.

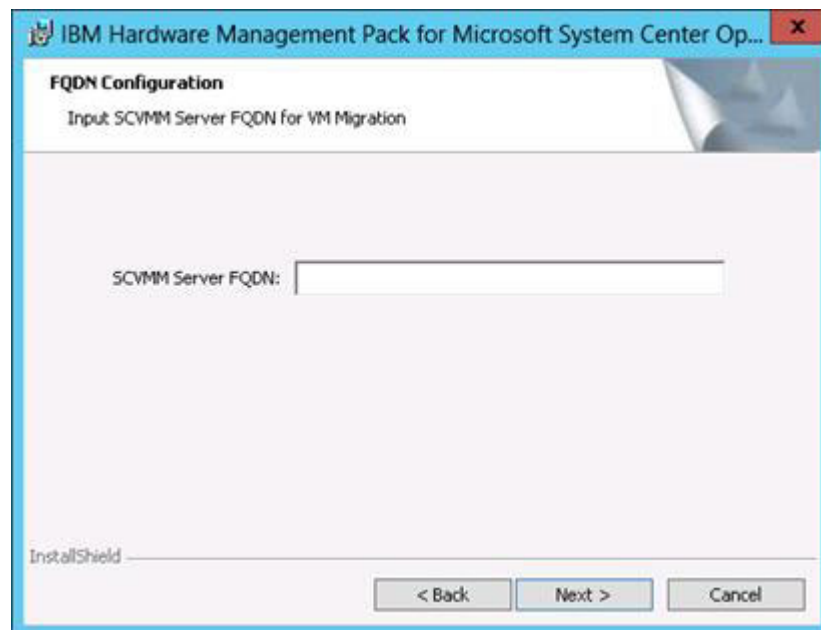


Figure 4. SCVMM Server FQDN Configuration

8. If your system had a previous installation of IBM Hardware Management Pack, the Program Maintenance page opens. Select one of the following options.

**Repair function:**

Reinstalls the code and registry entries on the local server.

If the system already has version v5.5 installed, you can select to repair or remove the IBM Hardware Management Pack code.

Verify the default target location. If necessary, select the target folder for the installation code and the knowledge articles that describe IBM systems and components.

**Remove function:**

Uninstalls the IBM Hardware Management Pack package from the local system but does not delete the management packs from the Operations Manager.

Use the Operations Manager Console to delete the management packs from the Operations Manager.

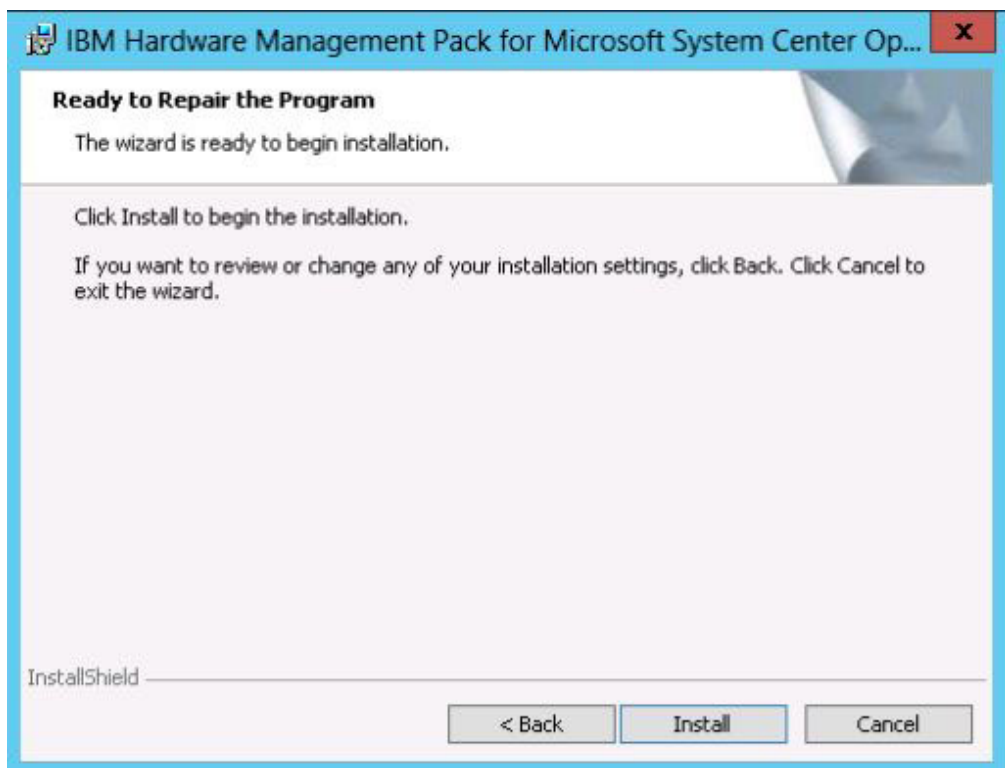


Figure 5. Ready to Repair Program

9. If you selected **Repair Function**, click **Install** to proceed with the repair. The Install/Repair/Remove Confirmation page opens.
10. Click **Next** to confirm the installation.  
If you are installing on a non-Root Management Server, you need to manually configure the Root Management Server name.
11. When the installation is finished, select **Read me** and **Import Management packs to the Operations Manager**, and then click **Finish**.

**Note:** Import management packs to Operations Manager is displayed when the software dependency is satisfied. When this option is not displayed, you must import the management packs manually. The imported management packs may not be visible from Operations Manager Console until the Operations Manager refreshes the management pack inventory data. If the Import management packs to Operations Manager is not displayed, perform the following steps to manually import the management packs.

12. Read the PostSetupCheckList.rtf file and take the suggested actions. The PostSetupCheckList.rtf file is installed in: %Program Files%\IBM\IBM Hardware Management Pack\.
13. Open the Operations Console of the Microsoft System Center Operations Manager to import the management packs of the IBM Hardware Management Pack to the Operations Manager.
14. Click the **Administration** button, right-click **Management Packs**, and then click **Import Management Packs**.
15. Follow the wizard directions to manually import the five management packs of the IBM Hardware Management Pack. By default, the management packs are installed in %ProgramFiles%\IBM\IBM Hardware Management Pack\Management Packs

## **IBM Hardware Management Packs**

After the IBM Hardware Management Packs are successfully imported, the IBM Hardware Management Packs listed below will display in the Administration pane of the Operations Manager Console.

For Microsoft System Center Operations Manager 2012, the IBM Hardware Management Packs are:

### **IBM Hardware Management Pack - Common Library:**

IBM.HardwareMgmtPack.Common.mp

### **IBM Hardware Management Pack for IBM System x and x86/x64 Blade Systems:**

IBM.HardwareMgmtPack.xSystems.mp

### **IBM Hardware Management Pack for IBM BladeCenter Chassis and Modules:**

IBM.HardwareMgmtPack.BladeCenter.v2.mp

### **IBM Hardware Management Pack – Hardware IDs Library:**

IBM.HardwareMgmtPack.HardwareIDs.mp

### **IBM Hardware Management Pack - Relation Library:**

IBM.HardwareMgmtPack.Relation.v2.mp

### **IBM Hardware Management Pack for IBM Flex System Chassis and Modules:**

IBM.HardwareMgmtPack.FlexSystem.v2.mp

### **IBM Hardware Management Pack - Flex Relation Library:**

IBM.HardwareMgmtPack.RelationCMM.v2.mp

**IBM Hardware Management Pack for IBM Integrated Management Module:**  
IBM.HardwareMgmtPack.IMM2.v2.mp

For Microsoft System Center Operations Manager 2007, the IBM Hardware Management Packs are:

**IBM Hardware Management Pack - Common Library:**  
IBM.HardwareMgmtPack.Common.mp

**IBM Hardware Management Pack for IBM System x and x86/x64 Blade Systems:**  
IBM.HardwareMgmtPack.xSystems.mp

**IBM Hardware Management Pack for IBM BladeCenter Chassis and Modules:**  
IBM.HardwareMgmtPack.BladeCenter.mp

**IBM Hardware Management Pack – Hardware IDs Library:**  
IBM.HardwareMgmtPack.HardwareIDs.mp

**IBM Hardware Management Pack - Relation Library:**  
IBM.HardwareMgmtPack.Relation.mp

**IBM Hardware Management Pack for IBM Flex System Chassis and Modules:**  
IBM.HardwareMgmtPack.FlexSystem.mp

**IBM Hardware Management Pack - Flex Relation Library:**  
IBM.HardwareMgmtPack.RelationCMM.mp

**IBM Hardware Management Pack for IBM Integrated Management Module:**  
IBM.HardwareMgmtPack.IMM2.mp

**Note:** Sometimes management pack entries do not display immediately after the installation. Refresh the window by pressing **F5**, or wait a few minutes for the management pack entries to display.

---

## Installing on more than one management server

The following procedure describes how to install the IBM Hardware Management Pack on more than one management server.

### Procedure

1. Install the IBM Hardware Management Pack on all the required management servers for your system.
2. Import the management packs on one of the management servers to the Operations Manager.

**Note:** To manage more than one BladeCenter in disjoint networks, install the IBM Hardware Management Pack on more than one management server. This enables communication with the respective BladeCenters by using SNMP. A management server can manage more than one BladeCenter chassis as long as the management server can use SNMP to communicate with the target chassis. For more detailed information about importing management packs, refer to the documentation for Operations Manager 2007 or 2012.



---

## Installing IBM Power CIM Provider

Installation of the IBM Power CIM Provider premium feature is optional. This feature enables power management on power-capable target systems.

### Before you begin

Power management is a premium feature that requires the purchase of an activation license. For details about obtaining an activation license, contact your IBM sales representative.

For a list of IBM server that provide power management capabilities, see “Supported IBM servers” on page 5.

### About this task

Unlike the IBM Hardware Management Pack installation, the IBM Power CIM Provider installation must be performed on every endpoint where power management functionality is desired.

### Procedure

- The file name of the IBM Power CIM Provider installer is `IBMPowerCIMInstaller.msi`.  
By default, the installer file is in the toolbox directory: `%ProgramFiles%\IBM\IBM Hardware Management Pack\toolbox`.
- To run an automated silent installation of the IBM Power CIM Provider without user interface prompting, execute the following command: **`msiexec /qn /i IBMPowerCIMInstaller.msi`**.  
The user interface level of the installation program can be controlled with standard `msiexec` command-line parameters.
- Similarly, to run a silent uninstallation of the IBM Power CIM Provider, execute the following command: **`msiexec /qn /x IBMPowerCIMInstaller.msi`**.  
When the installation is run in silent mode, the default folder location `C:\Program Files\IBM\IBM Power CIM Provider\` is used as the target for all installation files.
- The IBM Power CIM Provider installer executes a customizable action batch script during the installation process to register the provider with the IBM Director Platform Agent CIM server.  
If any errors occur while running this script, the details of the errors are logged to a file called `RegIBMPowerCIM.log` in the IBM Power CIM Provider installation directory. Consult this file for more detailed information about installation and uninstallation results.
- Do not run more than one instance of the Power CIM installer at a time.  
IBM Power CIM installer does not detect multiple simultaneous installation instances of itself.

---

## Installing the IBM License Tool and activating the premium features

To activate the premium features, System Center Operations Manager (SCOM) UIM requires that you activate the license on the System Center Operations Manager server only. It is not necessary to activate the license on each management target (client).

The license token is automatically delivered to the client when it is managed by a licensed SCOM server. For more information about activating the premium features, refer to the "*IBM Upward Integration for Microsoft System Center Installer Guide*".

---

## Upgrading to IBM Hardware Management Pack Version 5.5

If you start the installation process and discover that a prior version of the IBM Hardware Management Pack is installed already, the installation program automatically performs an upgrade of the IBM Hardware Management Pack.

To upgrade to version 5.5, on the Operations Manager console, place the management server where you are installing the IBM Hardware Management Pack in maintenance mode. Keep the management server in maintenance mode until you finish importing the new management pack.

**Note:** When upgrading from v4.5, the *automatic import MP* function may not import the new management pack. The program cannot identify whether there was an upgrade or a failure in the previous installation. Since a new management pack is introduced in v5.0 or higher, you will need to manually import the management pack when upgrading from v4.5.

### Upgrading more than one management server

If you are installing the IBM Hardware Management Pack on more than one management server, finish installing the IBM Hardware Management Pack on all of the management servers completely before importing the management packs. When the installation is finished, take the management servers out of maintenance mode.

---

## Uninstalling the IBM Hardware Management Pack, version 5.5

The following procedure describes how to uninstall the IBM Hardware Management Pack.

### Procedure

1. Place the server from which you are uninstalling the IBM Hardware Management Pack, into maintenance mode.

2. Remove the management pack entries from the Operations Manager Console of the Microsoft System Center Operations Manager. For more information, see “Deleting the IBM Hardware Management Packs.”
3. Use **Add or Remove Programs** to remove the IBM Hardware Management Pack.

---

## Deleting the IBM Hardware Management Packs

To prevent errors caused by missing runtime support libraries, delete the management packs from the Operations Manager first before removing the IBM Hardware Management Pack package. Errors can also occur if you uninstall the IBM Hardware Management Pack from more than one management server.

### Before you begin

If you plan to continue using the IBM Hardware Management Pack, but only need to move the responsibility of one management server to another server, make sure that a new designated management server has taken over the responsibility successfully before you remove the installed package of the IBM Hardware Management Pack.

### Procedure

1. In the Administration pane of the Operations Manager Console, select and delete the following management pack entries of the IBM Hardware Management Pack from Operations Manager:
  - IBM Hardware Management Pack – Common Library
  - IBM Hardware Management Pack for IBM System x and x86/x64 Blade Systems
  - IBM Hardware Management Pack for IBM BladeCenter Chassis and Modules
  - IBM Hardware Management Pack – Hardware IDs Library
  - IBM Hardware Management Pack – Relation Library
  - IBM Hardware Management Pack for IBM Flex System Chassis and Modules
  - IBM Hardware Management Pack – Flex Relation Library
  - IBM Hardware Management Pack for IBM Integrated Management Module
2. Remove the software package and files as described in the “Uninstalling the software package” on page 30 section, by using the **Add/Remove Programs** option.

## Removing the IBM Power CIM Provider

The following procedure describes how to remove the IBM Power CIM Provider.

### About this task

To remove the IBM Power CIM Provider, perform step 1. Step 2 provides uninstallation results and debug information.

### Procedure

1. By using **Add/Remove Programs** on the managed server, select the IBM Power CIM Provider you want to remove, and click **uninstall**. The CIM Server, *wmicimserver* may take a few minutes to completely unload the IBM Power CIM Provider.
2. Check the IBM Power CIM Provider installation directory for a file called *RegIBMPowerCim.log*, which lists the output from the uninstallation process. This log file will indicate whether an error may have occurred during uninstallation.

#### Notes:

- To avoid unpredictable results, uninstall the IBM Power CIM Provider before uninstalling the IBM Director Agent.
- If you accidentally uninstall IBM Director Agent first, and then try uninstalling IBM Power CIM Provider, the IBM Power CIM Provider may not get uninstalled.

Complete the following steps.

- a. To uninstall IBM Power CIM Provider, reinstall IBM Director Agent, and repair the IBM Power CIM Provider.
- b. Uninstall IBM Power CIM Provider, and then uninstall the IBM Director Agent.

## Uninstalling the software package

The following procedure describes how to uninstall the IBM Hardware Management Pack.

### Procedure

1. Remove the management pack entries as described in “Deleting the IBM Hardware Management Packs” on page 29.
2. Uninstall the software package and files entirely by using **Add/Remove Programs** in the Windows Control panel, select **Remove the IBM Hardware Management Pack for Microsoft System Center Operations Manager 2007, v5.5**.

## Downgrading to a previous version

To downgrade the IBM Hardware Management Pack to a previous version, uninstall the current version and reinstall the earlier version.

---

## Reinstalling IBM Hardware Management Pack, version 5.5

If you recently removed management packs from the Microsoft System Center Operations Manager console, you will need to wait for the settings to be propagated to the Operations Manager Console database before you can reinstall.

**Important:** If you do not wait for the removal of the management packs to register, reinstalling can result in managed clients not being listed on the Operations Manager.

See Discovery information is missing after you delete and then reimport a management pack in Microsoft System Center Operations Manager 2007 for information about this known limitation for Microsoft System Center Operations Manager.

If you remove the management packs from the console, you detach the IBM Hardware Management Pack from the Microsoft System Center Operations Manager server. You must then reinstall the IBM Hardware Management Pack into Microsoft System Center Operations Manager and add the management packs back to the console view.

---

## Configuring BladeCenter SNMP settings

IBM BladeCenter chassis that are correctly enabled for SNMP can be discovered automatically by Microsoft network device discovery. After installing the IBM Hardware Management Pack, you can verify whether the BladeCenter chassis are discoverable.

### Procedure

1. To view the Microsoft System Center Operations Manager consoles that discover BladeCenter chassis, click **IBM Hardware > IBM BladeCenters and Modules > Windows Computers for managing IBM BladeCenters**.

Use this view to identify the health of computers that have the IBM Hardware Management Pack installed and are able to discover and manage BladeCenter chassis and components.

2. To monitor IBM(r)BladeCenter(r)s and modules, click **Monitoring > IBM Hardware > IBM BladeCenter(s) and Modules**.

Chassis units are displayed in the results pane followed by a view of their components which is organized in the same way that the management modules present components:

- IBM BladeCenter Blades
- IBM BladeCenter Chassis
- IBM BladeCenter Cooling Modules
- IBM BladeCenter I/O Modules
- IBM BladeCenter Management Modules
- IBM BladeCenter Media Modules
- IBM BladeCenter Power Modules
- IBM BladeCenter Storage Modules

Each module type has a health state and the following properties:

- A product name and a logical name for blades
- A product name and a logical name for the module
- Physical location information

3. Log in to the IBM BladeCenter AMM web console.
4. To set ports for SNMP communication for a BladeCenter chassis that has not been discovered automatically, click **MM Control > Port Assignment** on the management module web console.




Figure 6. Default SNMP ports

Use the default SNMP ports of **161** for agent (queries/polling) and **162** for trapping. It is important for the SNMP port settings to be consistent. Otherwise, the Operations Manager cannot discover the BladeCenter chassis.

5. To change the SNMP settings, click **MM Control > Network Protocols > Simple Network Management Protocol SNMP** and complete the following steps.
  - a. Select **Enabled for SNMP Traps, SNMP v1 agent**.

Table 12. SNMP settings

Community name	Access type	Fully qualified host name or IP address
Public	Set	yourOpsMgrServer.yoursite.yourcompany.com

- b. Enter the following information for each Microsoft System Center Operations Manager management server that manages the BladeCenter:
  - **Community name** is assigned to the BladeCenter through which SNMP communicates.
  - The **Fully qualified host name or the IP address**.
- c. From the **Access type** list, select **Set**. **Set** is the access type required for enabling the management tasks. A task example is remotely powering on or off a blade server through the Operations Manager Console.

If you do not intend to allow this type of task through the Operations Manager console. You can lower the access type to **Trap**. At a minimum, the **Trap** access type must be set for the Operations Manager server to perform SNMP queries and receive SNMP traps from the BladeCenter.

To receive events from management modules, a network connection must exist between the management module and the Microsoft System Center Operations Manager. You must also configure the management module to send events.



6. To enable alerts using SNMP over the LAN in firmware revision 46, click **MM Control > Alerts**. In the right pane, under **Remote Alert Recipients**, click the **not used** link to configure the alert recipient as illustrated in the next figure. This step might vary slightly depending on the firmware level.

---

### Remote Alert Recipient 3

1. If you enable a SNMP over LAN recipient, you also need to complete the SNMP section on the [Network Protocols](#) page.
2. If you enable an E-mail over LAN recipient, you also need to complete the SMTP section on the [Network Protocols](#) page.

By entering an email or SNMP address not assigned to your company, you are consenting to share hardware serviceable events and data with the owner of that email or SNMP address not assigned to your company. In sharing this information, you warrant that you are in compliance with all import/export laws.

Status	Disabled 
Name	<input type="text"/>
Notification method	SNMP over LAN 
Receives critical alerts only	<input type="checkbox"/>

---

Figure 7. Enabling alerts using SNMP



- a. In the new Remote Alert Recipient window, change the status from **Disabled** to **Enabled**.
- b. In the **Name** field, enter a descriptive name for the management server for Microsoft System Center Operations Manager that you will be using to manage the BladeCenter. See “Discovering a BladeCenter in Operations Manager 2007” on page 34 for more about the Management Server setting.
- c. From the **Notification method** list, select **SNMP over LAN**.
- d. Click **Save**. The following figure is an example of a completed Remote Alert Recipient.

---

### Remote Alert Recipient 3

1. If you enable a SNMP over LAN recipient, you also need to complete the SNMP section on the [Network Protocols](#) page.
2. If you enable an E-mail over LAN recipient, you also need to complete the SMTP section on the [Network Protocols](#) page.

By entering an email or SNMP address not assigned to your company, you are consenting to share hardware serviceable events and data with the owner of that email or SNMP address not assigned to your company. In sharing this information, you warrant that you are in compliance with all import/export laws.


Status	Enabled 
Name	SCOM_RSM_01
Notification method	SNMP over LAN 
Receives critical alerts only	<input type="checkbox"/>

---

Figure 8. Remote Alert Recipient

7. Complete the following instructions for firmware revision 46:
  - a. In the navigation pane, under **MM Control**, click **Alerts**.
  - b. From the context menu, select **Monitor Alerts**.
  - c. Select the alerts to send, and click **Save**.

The following figure provides an example of what is displayed after completing this task.

**Monitored Alerts** 

Use enhanced alert categories

	<input checked="" type="checkbox"/> Critical Alerts	<input checked="" type="checkbox"/> Warning Alerts	<input checked="" type="checkbox"/> Informational Alerts
Chassis/System Management	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Cooling Devices	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Power Modules	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Blades	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
I/O Modules	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Storage Modules	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Event Log		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Power On/Off			<input checked="" type="checkbox"/>
Inventory change			<input checked="" type="checkbox"/>
Network change			<input checked="" type="checkbox"/>
User activity			<input checked="" type="checkbox"/>

Figure 9. Monitored alerts

## Discovering a BladeCenter in Operations Manager 2007

The following procedure describes how to discover a BladeCenter in Operations Manager 2007.

### About this task

Log in to the Microsoft System Center Operations Manager operations console as Administrator.

### Procedure

1. In navigation pane, click **Administration > Device Management > Agent Managed > Discovery Wizard** to start the Computers and Device Management Wizard.



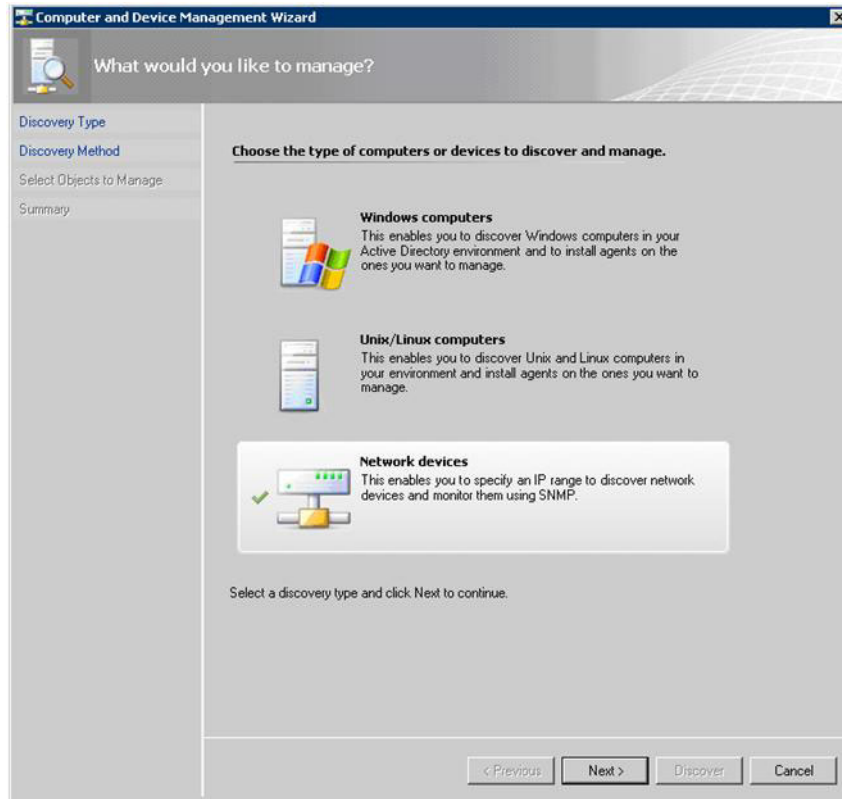


Figure 10. Discovery Wizard

2. On the What would you like to manage page, click **Network devices** and click **Next**, as shown in the figure above for Microsoft System Center Operations Manager 2007 R2.

**Note:** For Microsoft System Center Operations Manager 2007 SP1, make the following selections:

- a. Click **Advanced discovery** for the **Auto or Advanced?**.
- b. Click **Network Devices for Computer & Device Types**.
- c. From the **Management Server** list, select the management server that will discover and manage the BladeCenter.

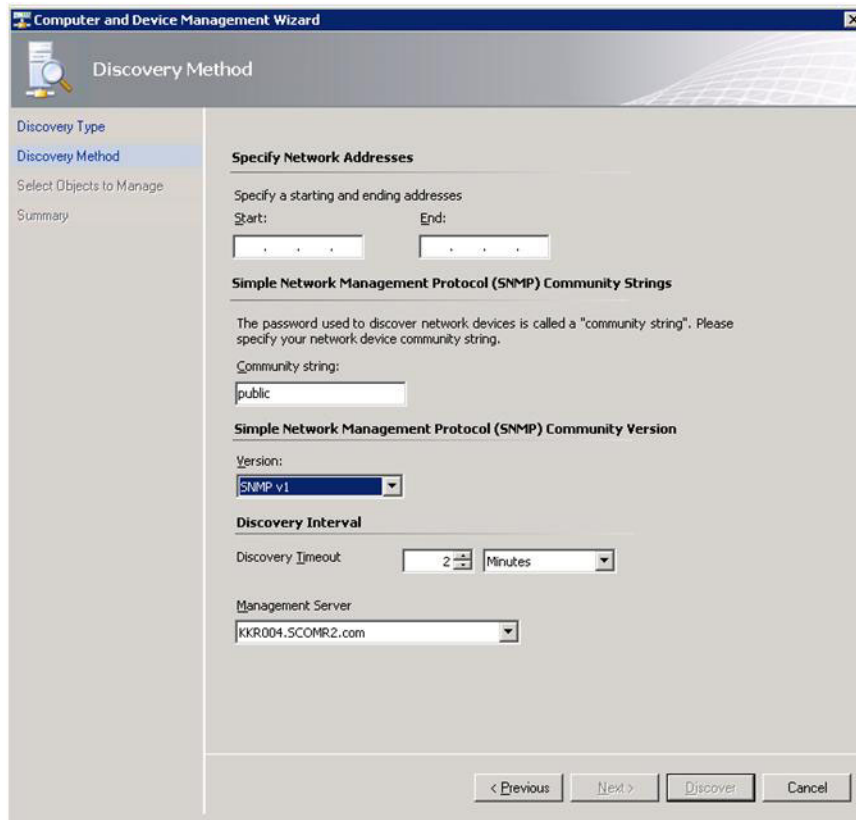


Figure 11. Discovery Method

3. On the Discovery Method page, enter the following information:
  - a. **Specify Network Addresses:** Provide an IP address range for discovery. Enter the **start** and **end** IP addresses.
  - b. **Community String:** Enter the name used on the chassis SNMP settings.
  - c. **Version:** From the **Version** list, select **SNMPv1**.
  - d. **Discovery Interval:** Select the Discovery Timeout, selecting the timeout number of minutes.
  - e. **Management Server:** Select the Microsoft System Center Operations Manager management server that will discover and manage the target BladeCenter.

**Note:** Ensure the management server that has the IBM Hardware Management Pack installed is also set up to discover and manage the target chassis through its SNMP settings. For more information, see “Configuring BladeCenter SNMP settings” on page 31 and “Discovering an IBM Flex System Chassis enabled for SNMP” on page 45.

- f. Click **Discovery** to open the Select Objects to Manage page.

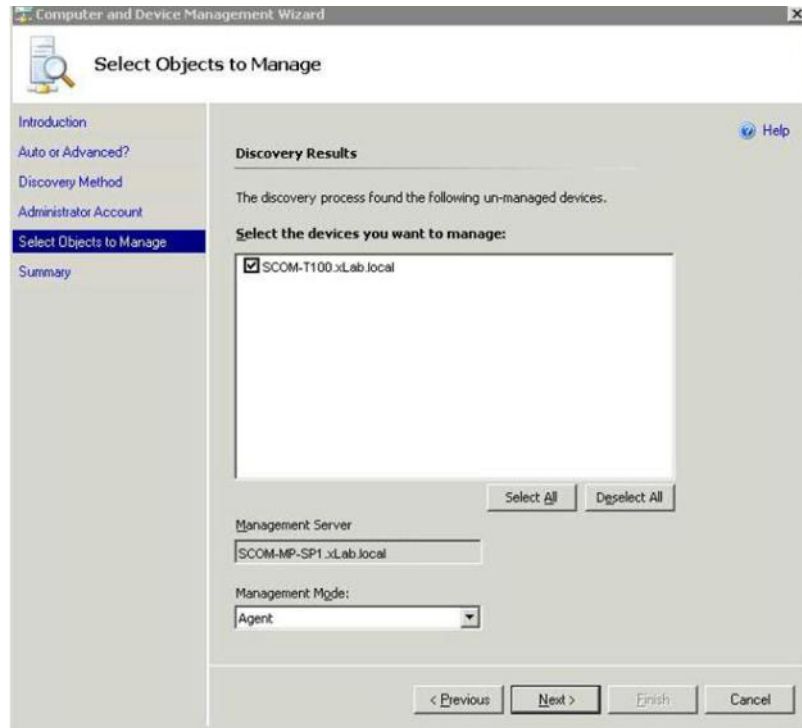


Figure 12. Select Objects to Manage

4. Complete the following steps, and then click **Next**.
  - a. **Select the devices you want to manage:** Select the IP address of the chassis unit to manage.
  - b. **Management Server:** Accept the default values.
  - c. **Management Mode:** Accept the default values.

**Note:** For Microsoft System Center Operations Manager 2007 SP1, enter the name of the Microsoft System Center Operations Manager Management Server that you entered in the **Proxy Agent** field on the Auto or Advanced page.

## Discovering a BladeCenter in Operations Manager 2012

The following procedure describes how to discover a BladeCenter in Operations Manager 2012.

## About this task

Log in to the Microsoft System Center Operations Manager operations console as Administrator.

## Procedure

1. In the navigation pane, click **Administration > Device Management > Agent Managed > Discovery Wizard** to start the Computers and Device Management Wizard.
2. In the navigation pane, click **Discovery Types**.

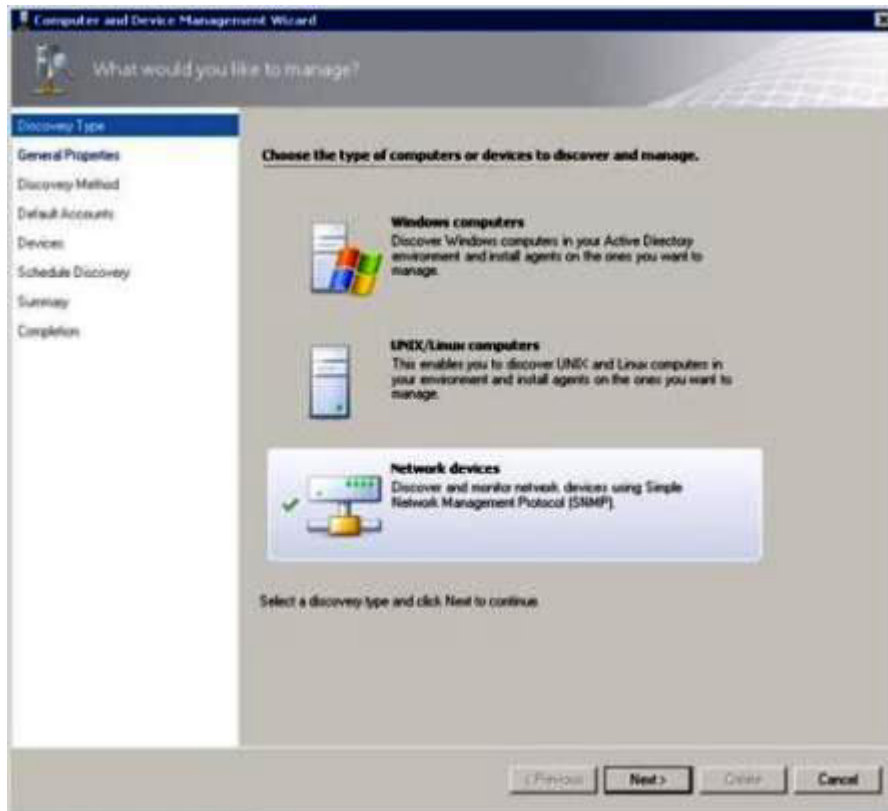


Figure 13. Discovery types

3. On the What would you like to manage page, click **Network devices** and click **Next**, as shown in the figure above for Microsoft System Center Operations Manager 2012.

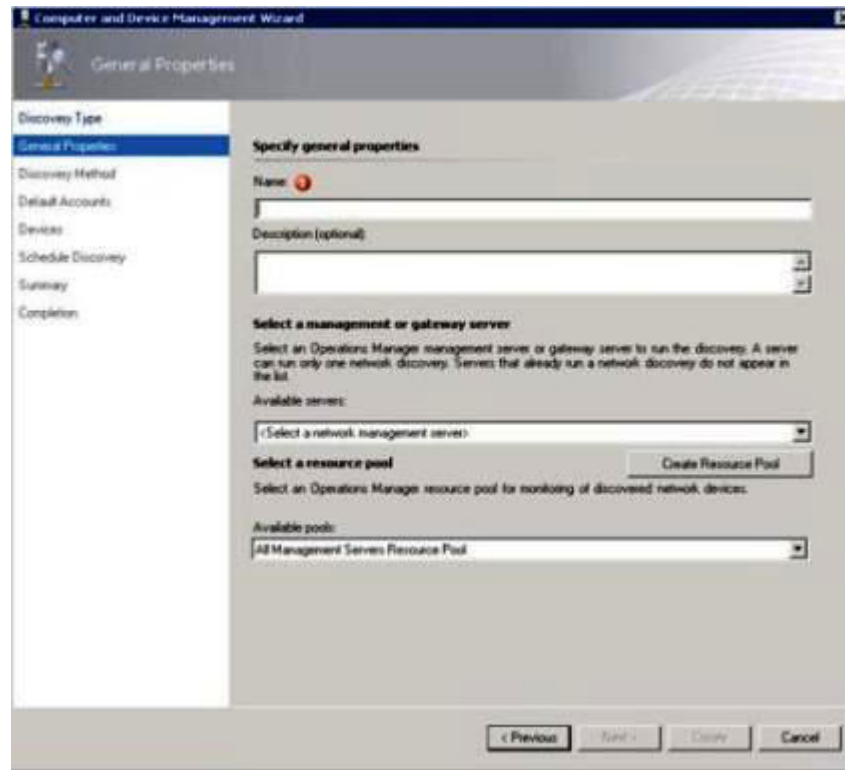


Figure 14. General Properties page

4. On the General Properties page, complete the following steps, and then click **Next**:
  - a. In the **Name** field, enter the name of the discovery rule.
  - b. Select **Available management server**.
  - c. Select **Resource pool**
5. On the Discovery Method page, select **Explicit Discovery** and click **Next**.
6. On the Default Accounts page, select **Create Account** and click **Finish** to create the community string. The Create Run As Account Wizard starts, and the Introduction page opens.

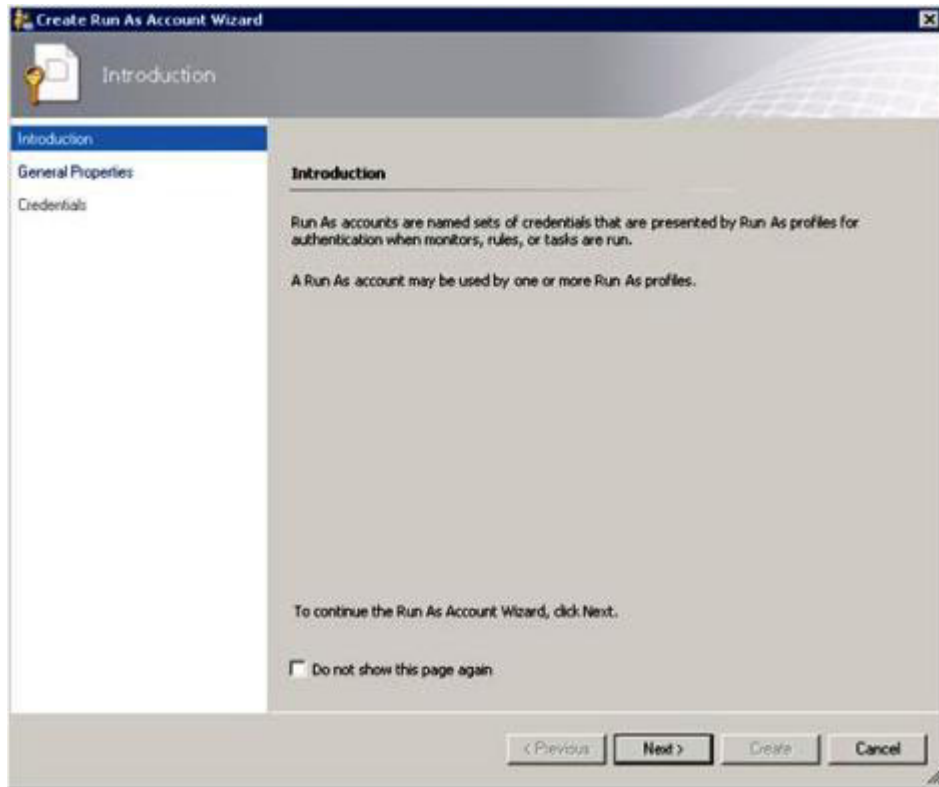


Figure 15. Introduction

7. On the Introduction page, click **Next**. The Devices page opens.

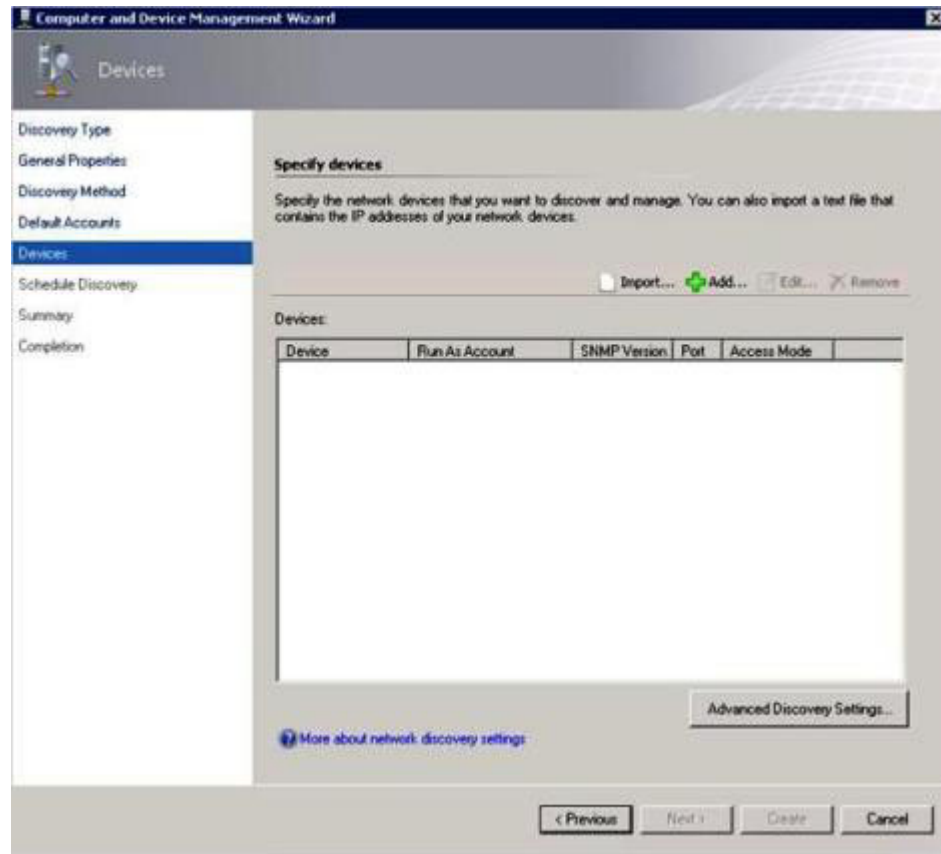


Figure 16. Devices

8. On the Devices page, click **Add**. The Add a Device dialog box opens.
9. In the Add a Device dialog box, complete the following steps:
  - a. In the **BladeCenter IP address** field, enter the IP address of the BladeCenter.
  - b. From the **Access Mode** list, select **SNMP**.
  - c. In the **SNMP V1 or V2 Run as account** field, change the value for SNMPV1 or SNMPV2.
  - d. Click **OK** to return to the Discovery Wizard.
 If you have additional devices to add, repeat step 8.
10. Click **Next** to finish the Discovery Wizard.

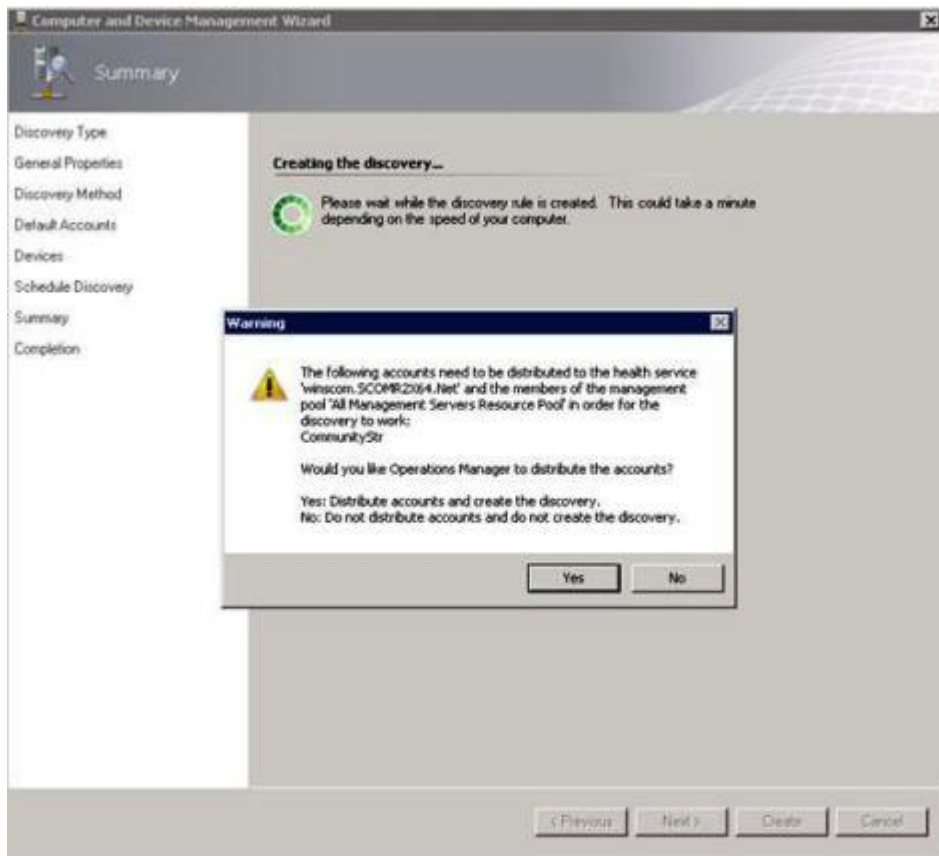


Figure 17. Creating the discovery warning

**Note:** If a Warning window opens asking if you would like to distribute the accounts, select **Yes** to finish the Discovery Wizard. The Completion page opens.



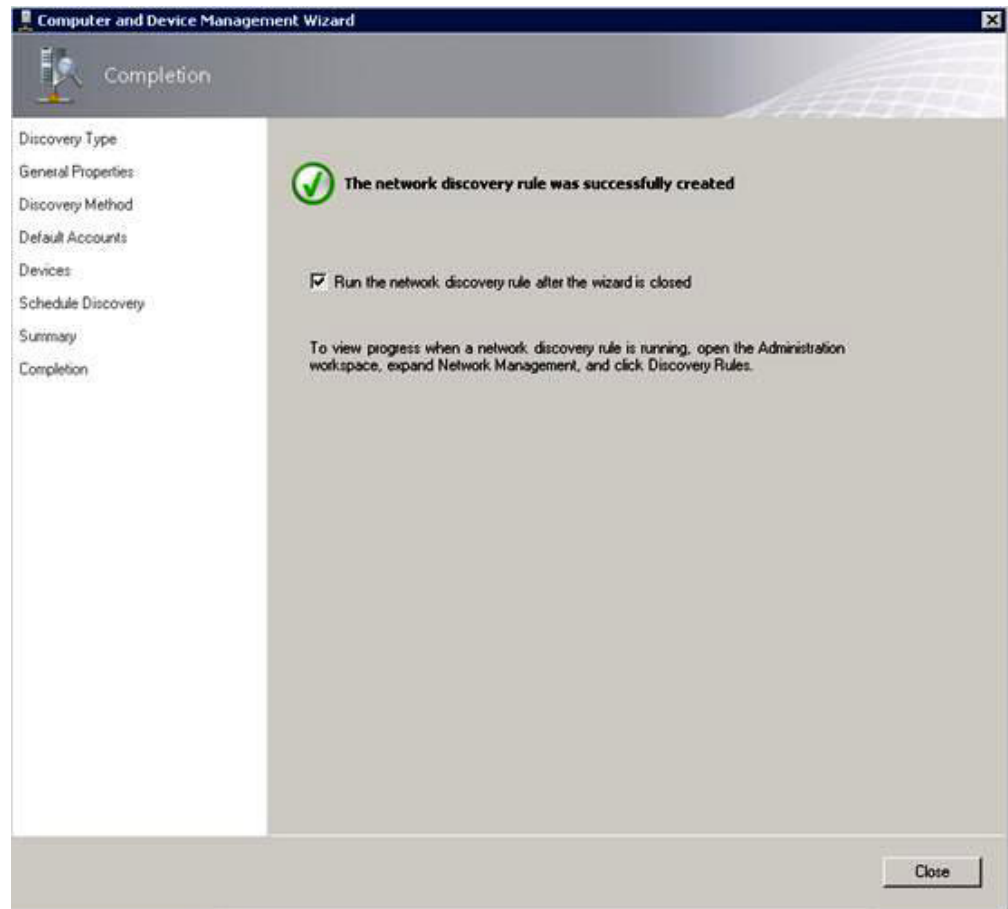


Figure 18. Discovery Wizard Completion

11. On the Completion page, select one of the following options:
  - Click **Run the network discovery rule after the wizard is closed** and click **Close**. The progress of a network discovery rule running after the Discovery Wizard is closed opens.
  - Click **Close**, and go to the Discovery Rules page to select a Discovery Rule to run.

The Discovery Rules page opens.

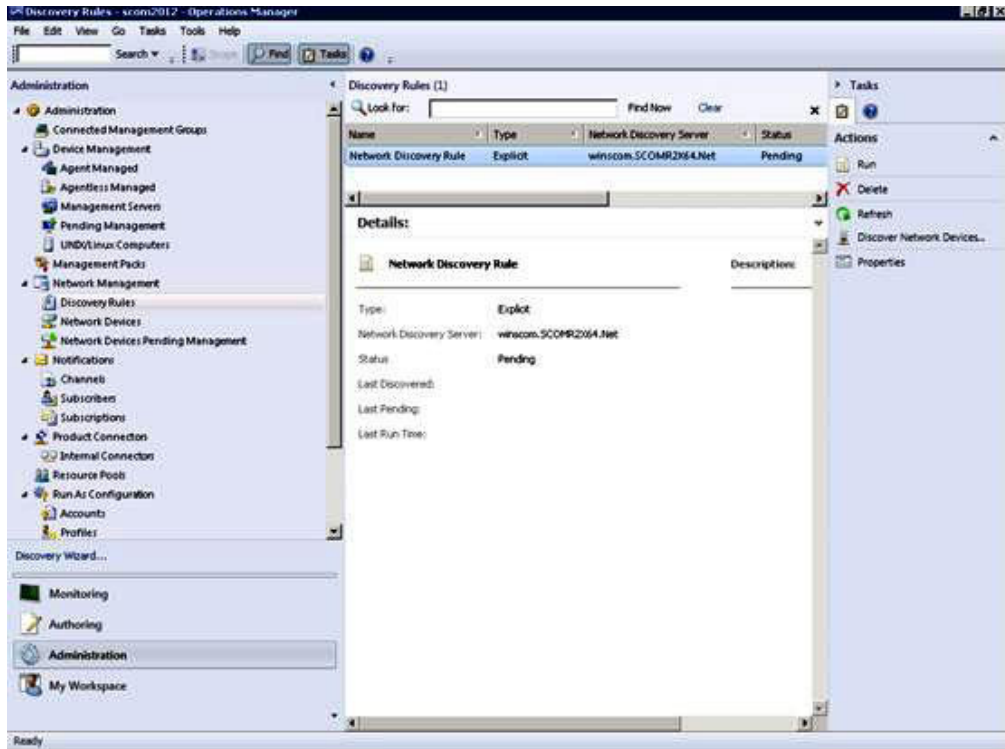


Figure 19. Discovery Rules

12. Select a **Discovery Rule** and click **Run**.

## Removing a discovered BladeCenter chassis

The following procedure describes how to remove a discovered BladeCenter chassis from a group of discovered systems.

### Before you begin

Log in to the Microsoft System Center Operations Manager operations console as Administrator.

### Procedure

1. Click **Administration > Device Management > Network Devices**. A list of BladeCenter chassis is displayed in the results pane.
2. Right-click a BladeCenter chassis and select **Delete** to start the delete task.

When the chassis and its discovered components are removed from the group, the following components are no longer displayed for the BladeCenter that was deleted:

- IBM BladeCenter Blades
- IBM BladeCenter Chassis
- IBM BladeCenter Cooling Modules
- IBM BladeCenter I/O Modules
- IBM BladeCenter Management Modules
- IBM BladeCenter Media Modules
- IBM BladeCenter Power Modules
- IBM BladeCenter Storage Modules

## Discovering an IBM Flex System Chassis enabled for SNMP

IBM Flex System Chassis that are correctly enabled for SNMP can be discovered automatically by the Microsoft network device discovery. After installing the IBM Hardware Management Pack, you can verify if the Flex System chassis are discoverable.

### Procedure

1. To discover a Flex System chassis, click **IBM Hardware > IBM Flex Systems and Modules > Windows Computers for managing IBM Flex Systems Chassis(s)**. You can also use this view to identify the health of computers that have the IBM Hardware Management Pack installed and to discover and manage the IBM Flex System Chassis and components.

**Note:** Only the management server that has the activation license installed can manage the IBM Flex System Chassis and modules.

2. To monitor IBM Flex System Chassis and modules, click **Monitoring > IBM Hardware > IBM Flex System Chassis(s) and Modules**. Chassis units are displayed in the results pane and include a view of their components organized in the same way that the management modules present components:

- IBM Flex System Compute Nodes/Storage
- IBM Flex System Cooling Modules
- IBM Flex System FanMux Modules
- IBM Flex System I/O Modules
- IBM Flex System Management Modules
- IBM Flex System Power Modules
- IBM Flex System RearLED Modules

Each module type has a health state and the following properties:

- A product name and a logical name for the module
- Physical location info

3. Log in to the IBM Flex System Chassis CMM web console. To set SNMP communication ports for an IBM Flex System Chassis, that has not been discovered automatically, click **Mgt Module Management > Network > Port Assignments on the Chassis management module web console**.

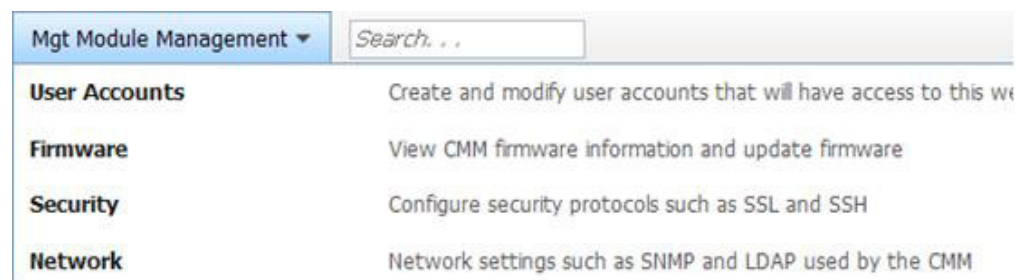


Figure 20. Default SNMP ports

It is important for the SNMP port settings to be consistent. Otherwise, the Operations Manager cannot discover the Flex chassis. Use the following default SNMP ports:

- 161 for agent (queries/polling)
- 162 for trapping

Serial Port	SNMP Agent	161
Port Assignments	SNMP Traps	162
Network Interfaces		

Figure 21. Setting default SNMP ports

4. To change the SNMP settings, click **Mgt Module Management > Network > SNMP**. There are two SNMP agent versions that can be selected for the System Center Operations Manager (SCOM) to manage the Flex chassis. Select one of the following methods:

- Method 1: Enabled for SNMPv1 Agent
- Method 2: Enabled for SNMPv3 Agent

To receive events from the management modules, a network connection must exist between the management module and the Microsoft System Center Operations Manager, and you must also configure the management module to send events.

5. Using **SNMP over LAN**, click **Events > Event Recipients**.

Events ▾	Service and Support ▾	Chassis Management ▾	Mgt Module Management ▾
<b>Event Log</b>	Full log history of all events		
<b>Event Recipients</b>	Add and modify E-Mail, SNMP, and Syslog recipients		

Figure 22. Selecting Event Recipients

6. Click **Create > Create SNMP Recipient**.

## Event Recipients

Create ▾	Delete	Global Settings	Syslog Settings	Generate Test Event
Create E-mail Recipient		Notification Method	Events to Receive	Status
Create SNMP Recipient		SNMP over LAN	As defined in Global Settings	Disabled
		SNMP over LAN	As defined in Global Settings	Enabled
9.125.90.84		SNMP over LAN	As defined in Global Settings	Enabled
9.115.252.91		SNMP over LAN	As defined in Global Settings	Enabled

Figure 23. Create Event Recipients

7. In the Create SNMP Recipient dialog box, complete the following steps.
  - In the **Descriptive name** field, enter a name.
  - From the Status list, select **Enable this recipient**.
  - For **Events to Receive**, select **Use the global settings** or **Only receive critical alerts**.
  - Click **OK** to return to the Event Recipients page.

## Event Recipients

Create	Delete	Global Settings	Syslog Settings	Generate Test Event
Create E-mail Recipient Create SNMP Recipient		Notification Method	Events to Receive	Status
		E-mail over LAN	As defined in Global Settings	Disabled
		SNMP over LAN	As defined in Global Settings	Enabled
9.125.90.84		SNMP over LAN	As defined in Global Settings	Enabled
9.115.252.91		SNMP over LAN	As defined in Global Settings	Enabled

Figure 24. Creating an SNMP Recipient

8. If you selected, **Use the global settings**, the Event Recipient Global Settings dialog box is displayed.

Event Recipient Global Settings x

These settings will apply to all event recipients.

Retry limit:

Delay between attempts (minutes):

Send event log with e-mail notifications

	<input type="checkbox"/> Critical Events	<input type="checkbox"/> Warning Events	<input type="checkbox"/> Informational Events
Chassis/System Management	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Cooling Devices	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Power Modules	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Compute Nodes	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
I/O Modules	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Event Log		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>
Power On/Off			<input checked="" type="checkbox"/>
Inventory change			<input checked="" type="checkbox"/>
Network change			<input checked="" type="checkbox"/>
User activity			<input checked="" type="checkbox"/>

Figure 25. Event Recipient Global Settings

- Click **OK** to return to the Event Recipients page.

## Enabling SNMPv1 Agent

The following procedure describes how to enable the **Enabled for SNMPv1 Agent** protocol.

### Procedure

- Click **Enabled for SNMPv1 Agent**.

### Simple Network Management Protocol (SNMP)

Enable SNMPv1 Agent  
 Enable SNMPv3 Agent

Contact   Traps   **Communities**

Select communities to configure. At least one community must be configured.

Community 1	<input checked="" type="checkbox"/> Enable Community 2
Community name: public	Community name: test
Access type: Set	Access type: Set
Fully Qualified Hostnames or IP Addresses: 0.0.0.0 0::0 9.125.90.84	Fully Qualified Hostnames or IP A: 0.0.0.0 9.115.253.41 9.115.252.91

Figure 26. Simple Network Management Protocol (SNMP)

- Click the **Traps** tab and click **Enable SNMP Traps**.
- Click the **Communities** tab and complete the following steps for every Microsoft System Center Operations Manager management server that will manage the Flex System:
  - In the **Community name** field, enter the name that is assigned to the Flex System through which SNMP communicates.
  - From the **Access type** list, select **Set**. This is required for enabling the management tasks. If you do not intend to allow this type of task through the Operations Manager console, you can lower the access type to **Trap**. At a minimum, the **Trap** access type must be set so that the Operations Manager server can perform SNMP queries and receive SNMP traps from the Flex System.
  - From the **Fully Qualified Hostnames or the IP Addresses** lists, select the appropriate entries.

**Note:** By default, the Chassis module Security Policies level is Secure. At this level, SNMPv1 cannot be enabled. To use SNMPv1, change the security level to **Legacy**, by clicking **Mgt Module Management > Security > Security Policies >**

Legacy.

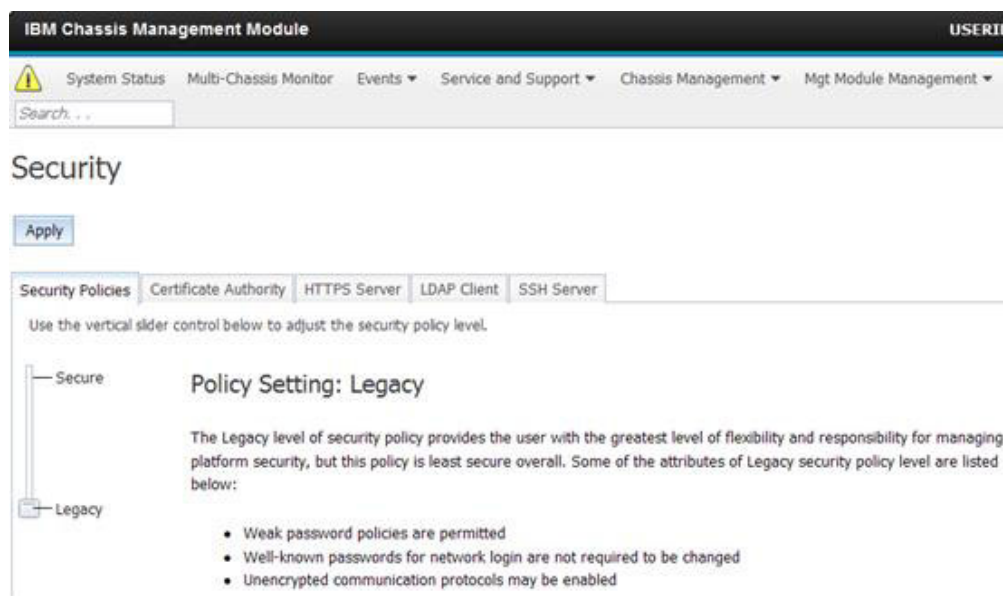


Figure 27. Security Policy setting

## Enabling SNMPv3 Agent

The following procedure describes how to enable the **Enabled for SNMPv3 Agent** protocol. Using SNMPv3 Agent requires that you either create a new user with the **Create User** option or use the default user.

### Before you begin

If you want to use SNMPv3 Agent to manage a Flex Chassis from the System Center Operations Manager (SCOM) server, you first need to create a SNMPv3 user account or select a default user from the list to open the User Properties page.

### Procedure

1. Click **Mgt Module Management > User Accounts**.
2. Click the **General** tab and set the user password.
3. Click the **SNMPv3** tab and configure the **Authentication Protocol**.

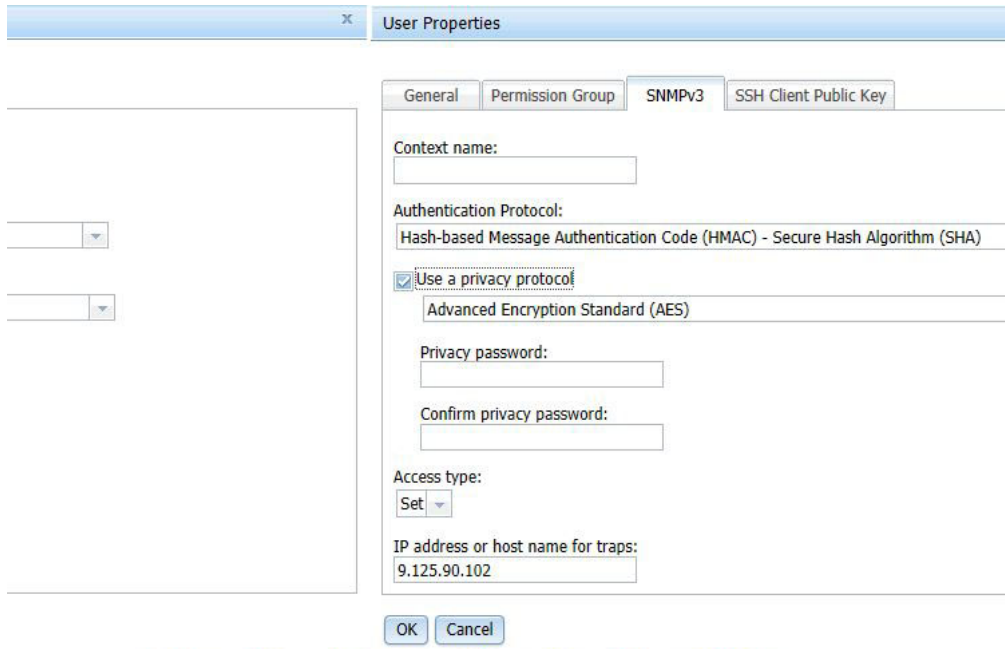


Figure 28. Account credentials for creating a new user for SNMPv3 devices

- a. From the **Authentication Protocol** list, select **Use a Privacy Protocol**.
  - b. In the **Privacy password** field, enter the authentication key, and in the **Confirm privacy password** field, re-enter the authentication key.
  - c. Change the **Access type** to **Set**.
  - d. In the **IP address or host name for traps** field, enter the SCOM server IP address.
4. Click **OK**.

## Discovering an IBM Flex System in Operations Manager 2007

Microsoft System Center Operations Manager 2007 only supports SNMPv1 for managing an IBM Flex System Chassis.

### About this task

To discover a chassis and its components in Microsoft System Center Operations Manager 2007, refer to “Discovering a BladeCenter in Operations Manager 2007” on page 34.



## Discovering an IBM Flex System in Operations Manager 2012

The following procedure describes how to discover an IBM Flex System in Microsoft System Center Operations Manager 2012.

### Before you begin

On a management server, log in to the Microsoft System Center Operations Manager operations console as Administrator.

**Note:** This feature only supports a CMM IP address. Do not use an IMM IP address.

### About this task

To discover a chassis and its components in Operations Manager 2012 using SNMPv1, refer to “Discovering a BladeCenter in Operations Manager 2007” on page 34.

To discover a chassis and its components in Operations Manager 2012 using SNMPv3, complete the following steps on a management server.

### Procedure

1. Click **Administration > Device Management > Agent Management > Discovery Wizard** to start the Computers and Device Management Wizard.
2. In the navigation pane, click **Discovery Types**.
3. On the What would you like to manage page, click **Network devices** and click **Next**.
4. On the General Properties page, complete the following steps:
  - a. In the **Name** field, enter the discovery rule.
  - b. Select an **Available management server**.
  - c. Select a **Resource Pool**.
5. On the Discovery Method page, select **Explicit Discovery** and click **Next**.
6. On the Default Accounts page, select **Next**.
7. On the Devices page, click **Add**. The Add a Device dialog box opens.
8. In the Add a Device dialog box, complete the following steps:
  - a. Enter the **Flex System IP address**.
  - b. Select **SNMP** for the Access mode.
  - c. Select **v3** for the SNMP version.
  - d. Select **Add SNMP V3 Run As Account**.
  - e. Perform the steps in the Create Run As Account Wizard to fill in the SNMPv3 account you just created in Flex Management web console.
  - f. Click **OK** to return to the Discovery Wizard.

If you have additional devices to add, repeat steps 7 and 8.

9. Click **Next** to complete the Discovery Wizard.
10. On the Completion page, select one of the following options:
  - Click **Run the network discovery rule after the wizard is closed** and then click **Close**. When the Discovery Wizard is closed, the progress of the network discovery rule running is displayed.
  - Click **Close**.
11. Select a **Discovery Rule** and click **Run**.

**Note:** You can also modify the discovery rule by selecting the rule's **Properties**.

## Removing a discovered IBM Flex System chassis

The following procedure describes how to remove a discovered IBM Flex System chassis from the group of discovered systems.

### Before you begin

Log in to the Microsoft System Center Operations Manager operations console.

### Procedure

1. Click **Administration > Network Devices**.
2. In the results pane, select the IBM Flex System or BladeCenter chassis you want to delete.
3. Right-click and select **Delete** to start the delete task.

When the chassis and its discovered components are removed from the group, the following components of an IBM Flex System chassis are no longer displayed:

- IBM Flex System Chassis Compute Nodes/Storage
- IBM Flex System Chassis Cooling Modules
- IBM Flex System Chassis FanMux Modules
- IBM Flex System Chassis I/O Modules
- IBM Flex System Chassis Management Modules
- IBM Flex System Chassis Power Modules
- IBM Flex System Chassis RearLED Modules

---

## Chapter 5. Working with the IBM Hardware Management Pack

The topics in this section describe how IBM Hardware Management Pack enhances the functionality of the Operations Manager by providing more detailed information about the managed IBM systems.

To learn more about using the Operations Manager when the IBM Hardware Management Pack is installed, perform the tasks in the “Monitoring through the Operations Manager Console” section.

The IBM Hardware Management Pack provides the following functions:

- Monitors the system using the Monitoring pane of the Operations Manager Console, as described in “Monitoring through the Operations Manager Console”
- Adds an IBM system to the managed systems, as described in “Adding an IBM system that will be managed by the Operations Manager” on page 61
- Monitors the health of systems, components, and systems-management software, as described in “Monitoring the health of systems, hardware components, and other targets” on page 72
- Identifies and resolves errors, as described in “Using Health Explorer to identify and resolve problems” on page 75
- Accesses the IBM knowledge pages, as described in “Using knowledge pages to resolve problems” on page 77

---

### Monitoring through the Operations Manager Console

The following procedure describes how to use the Operations Manager Console with the IBM Hardware Management Pack installed. After installing the IBM Hardware Management Pack, you can use the Monitoring pane of the Operations Manager Console to select folders and views that provide complete health information of your IBM BladeCenter chassis, Flex System Chassis and chassis components, and System x and x86/x64 blade servers. From the Operations Manager Console you can also discover IMM to enable and monitor Hardware Failure Management.

#### About this task

Perform these steps to become familiar with the Monitoring pane of the Operations Manager Console and the features that the IBM Hardware Management Pack adds:

#### Procedure

1. In the navigation pane, click the **Monitoring** tab. The Monitoring pane lists the systems and hardware components that you can monitor with the IBM Hardware Management Pack. The following figure shows a portion of the Monitoring pane after you install the IBM Hardware Management Pack.

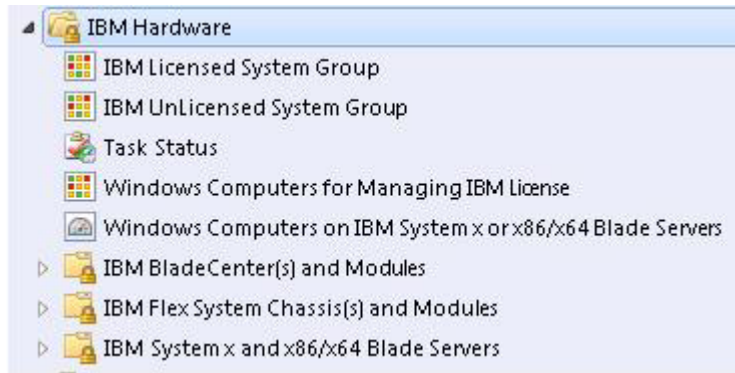


Figure 29. Monitoring pane

The IBM Hardware folder consists of several different views and folders that monitor data collected from IBM systems. The **Windows Computers on IBM System x or x86/x64 Blade Servers** view provides a global view. The other folders provide additional views of the different types of monitoring data collected from IBM systems.

**IBM Hardware:**

This folder includes active alerts, task status, and aggregate targets for all discovered IBM systems and hardware components.

**IBM Licensed System Group:**

This view provides the status of Windows computers on an IBM server when the premium features are enabled.

**IBM Unlicensed System Group:**

This view provides the status of Windows computers on the IBM server when the premium features are not enabled.

**Windows Computers for Managing IBM License:**

This view provides the status of Operations Manager management servers that are capable of managing the premium features.

**Windows Computers on IBM System x or x86/x64 Blade Servers:**

This view provides the status of IBM System x or x86/x64 Blade servers. Use this view as you would the **Monitoring > Computers** view. The difference is that this view contains only IBM System x or IBM BladeCenter x86/x64 blade servers.

**IBM BladeCenter(s) and Modules:**

This folder contains a summarized view of all IBM BladeCenters and Modules and personalized summary views of specific alerts, task status, IBM BladeCenters, and Windows computers for managing IBM BladeCenters.

**IBM Flex System Chassis and Modules:**

This folder contains a summarized view of all IBM Flex System Chassis and Modules and personalized summary views of specific alerts, task status, IBM Flex System Chassis, and Windows computers for managing IBM Flex System Chassis.

**IBM System x and x86/x64 Blade Servers:**

This folder contains a summarized view of all IBM systems including: IBM System x and BladeCenter x86/x64 Blade systems and personalized summary views of specific types of IBMSystem x and

BladeCenter x86/x64 Blade servers. These systems are grouped by platform type and include tower, rack, blade, enterprise server, and unclassified.

2. Click **Windows Computer on IBM System X or x86/x64 Blade Servers** to view detailed information from the Windows computers on IBM System x or x86/x64 Blade servers.

Only manageable hardware components are discovered and monitored, and therefore not all components are included. For example, a system with one or more non-manageable fans does not have all of its fans discovered or monitored. In the following figure, the detail view for the pane labeled IBM Hardware Components of IBMSystem x or x86/x64 Blade Servers shows various components.

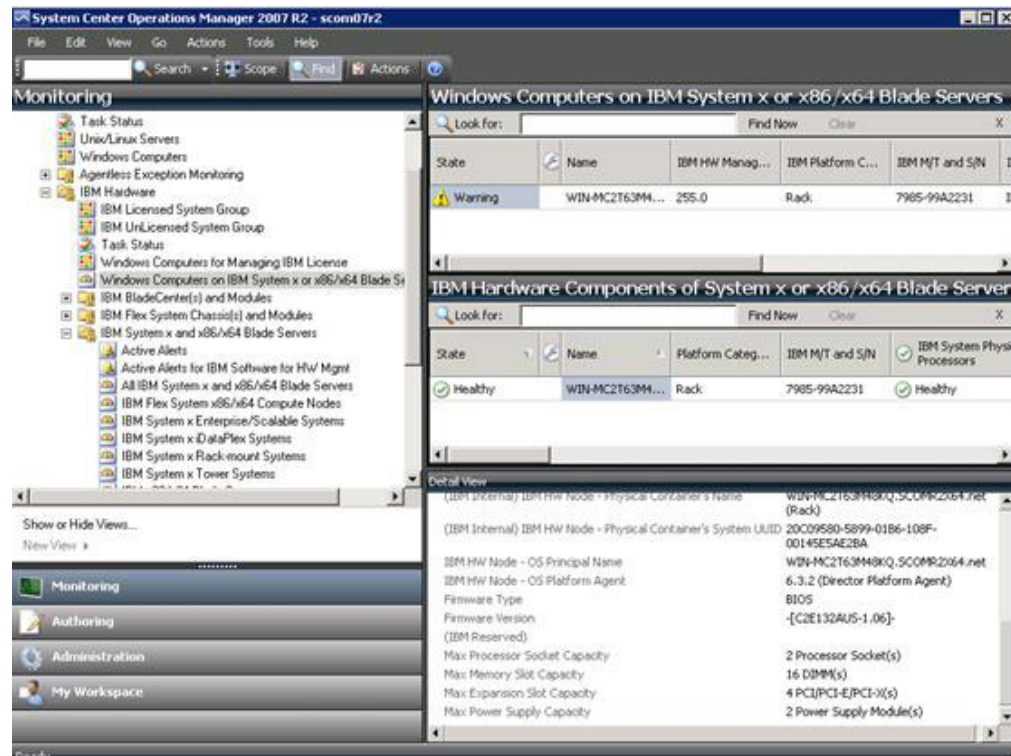


Figure 30. Windows Computers on IBM System x or x86/x64 Blade Server view

3. Click the **IBM BladeCenter(s) and Modules** folder to view detailed information about IBM BladeCenter(s) and modules.

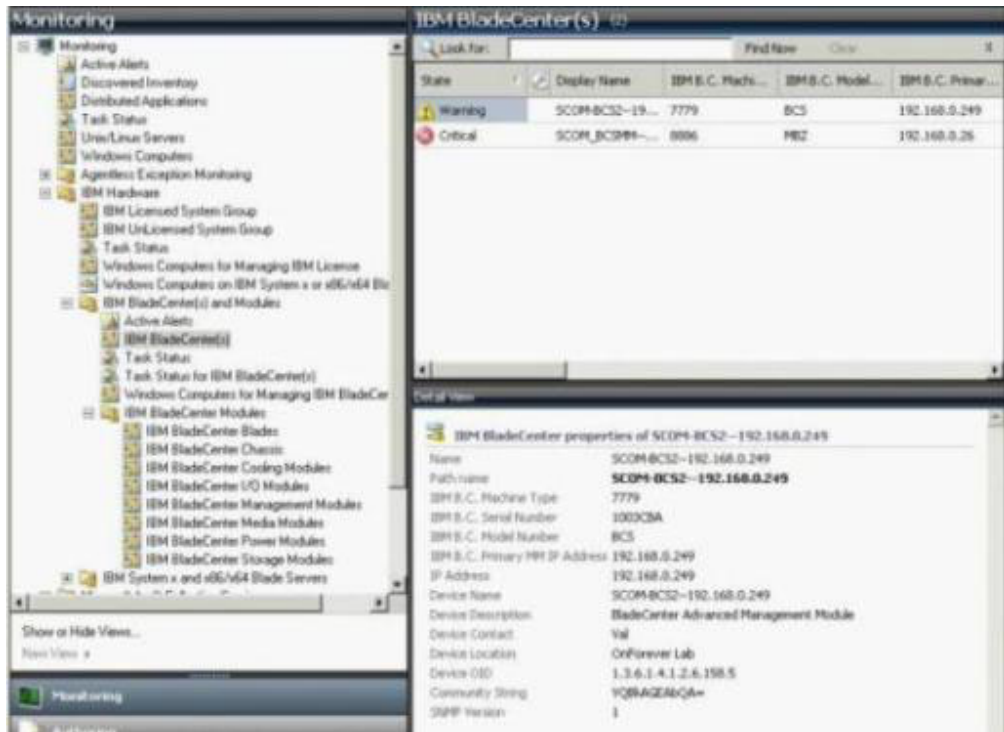


Figure 31. IBM BladeCenter(s) and Modules folder view

There are five views and one folder in the **IBM BladeCenter(s) Modules** folder:

**Active Alerts:**

This view provides the status of the IBM BladeCenter alerts.

**IBM BladeCenter(s):**

This view provides a summarized list of all IBM BladeCenter chassis and chassis components, such as Blades, Cooling, I/O, Storage, Power, Management Module, and other components.

**Task Status:**

This view provides the status of the IBM BladeCenters Modules and Chassis.

**Task Status for IBM BladeCenter(s):**

This view provides the status of the IBM BladeCenters.

**Windows Computers for Managing IBM BladeCenter(s):**

This view shows the management modules that can communicate with IBM BladeCenter chassis.

**IBM BladeCenter Modules:**

This folder contains all of the component information and status information for the BladeCenter chassis, chassis components, and blade servers. Categories include Blades, Chassis, Cooling, I/O, Management Module, Media Modules, Power, and Storage.

- Click the **IBM Flex System Chassis and Modules** folder to display detailed information about IBM Flex System Chassis and modules.

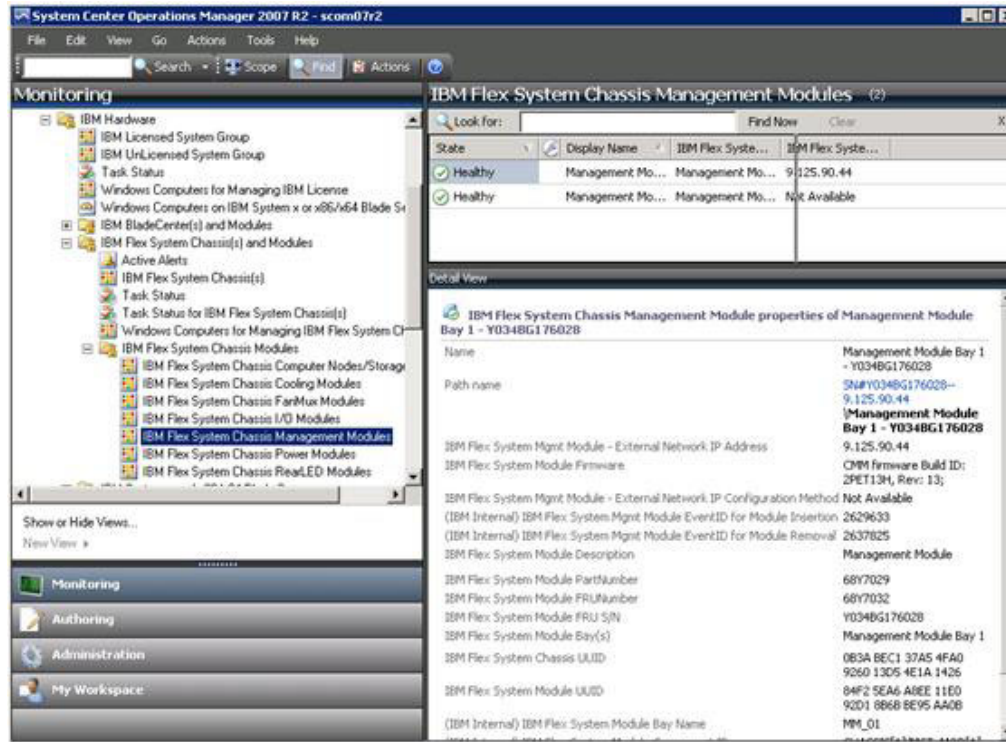


Figure 32. IBM Flex System Chassis folder view

There are five views and one folder in the IBM Flex System Chassis and Modules folder:

**Active Alerts:**

This view provides the status of the IBM Flex System Chassis alerts.

**IBM Flex System Chassis:**

This view provides a summarized list of all IBM Flex System Chassis and chassis components, such as Compute Node, Cooling, I/O, Storage, Power, Management Module, and other components.

**Task Status:**

This view provides the status of the IBM Flex system Modules and Chassis.

**Task Status for IBM Flex System Chassis:**

This view provides the status of the IBM Flex system chassis.

**Windows Computers for Managing IBM Flex System Chassis:**

This view shows management modules that can communicate with IBM Flex system chassis.

**IBM Flex System Chassis Modules:**

This folder contains all of the component information and status information for the Flex system chassis, chassis components, and compute nodes. Categories include Compute Node, Cooling, FanMux Modules, FSM, I/O Modules, Management Modules, Power Modules, Rear LED Modules, and Storage.

5. Click the **IBM Flex System Chassis Modules** folder to display the views in this folder. After discovering an IBM Flex System chassis and the chassis modules, the IBM Hardware Management Pack classifies the chassis modules according to their module type and then adds each module to the applicable module view:

- IBM Flex System Chassis Compute Nodes
- IBM Flex System Chassis Cooling Modules
- IBM Flex System Chassis FanMux Modules
- IBM Flex System Chassis FSM
- IBM Flex System Chassis I/O Modules
- IBM Flex System Chassis Management Modules
- IBM Flex System Chassis Power Modules
- IBM Flex System Chassis RearLED Modules
- IBM Flex System Chassis Storage

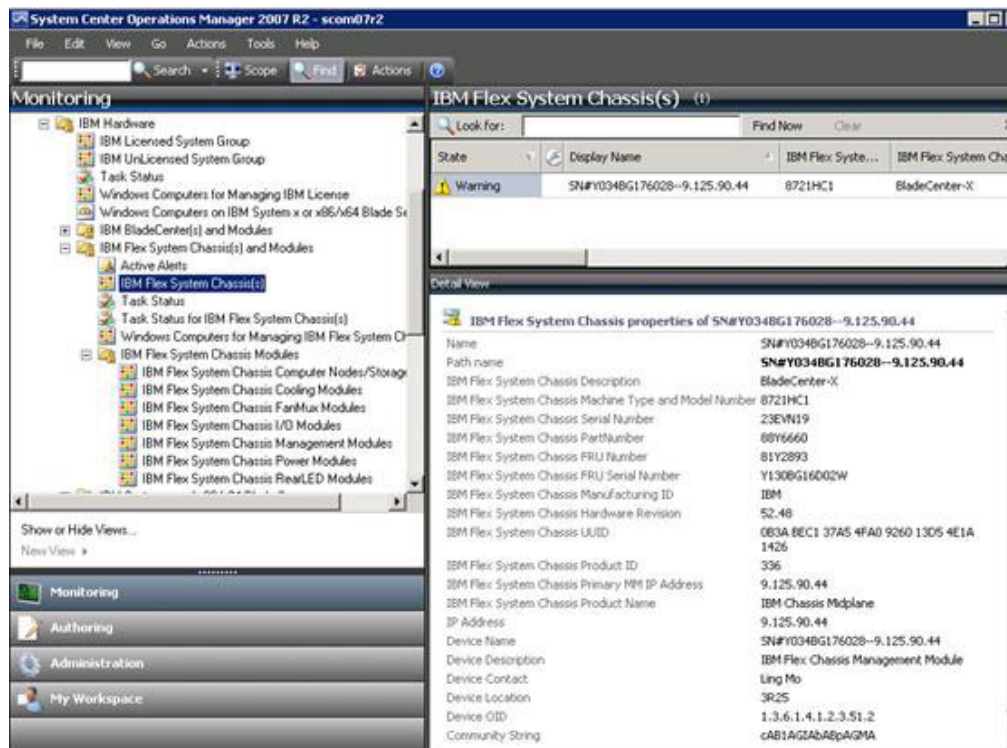


Figure 33. IBM Flex System Chassis Modules



6. Click the **IBM BladeCenter Modules** folder to display the views in this folder. After discovering an IBM BladeCenter chassis and its chassis modules, the IBM Hardware Management Pack classifies the modules according to their module type and then adds each module to the applicable module view:

- IBM BladeCenter Blades
- IBM BladeCenter Chassis
- IBM BladeCenter Cooling Modules
- IBM BladeCenter I/O Modules
- IBM BladeCenter Management Modules
- IBM BladeCenter Media Modules
- IBM BladeCenter Power Modules
- IBM BladeCenter Storage Modules

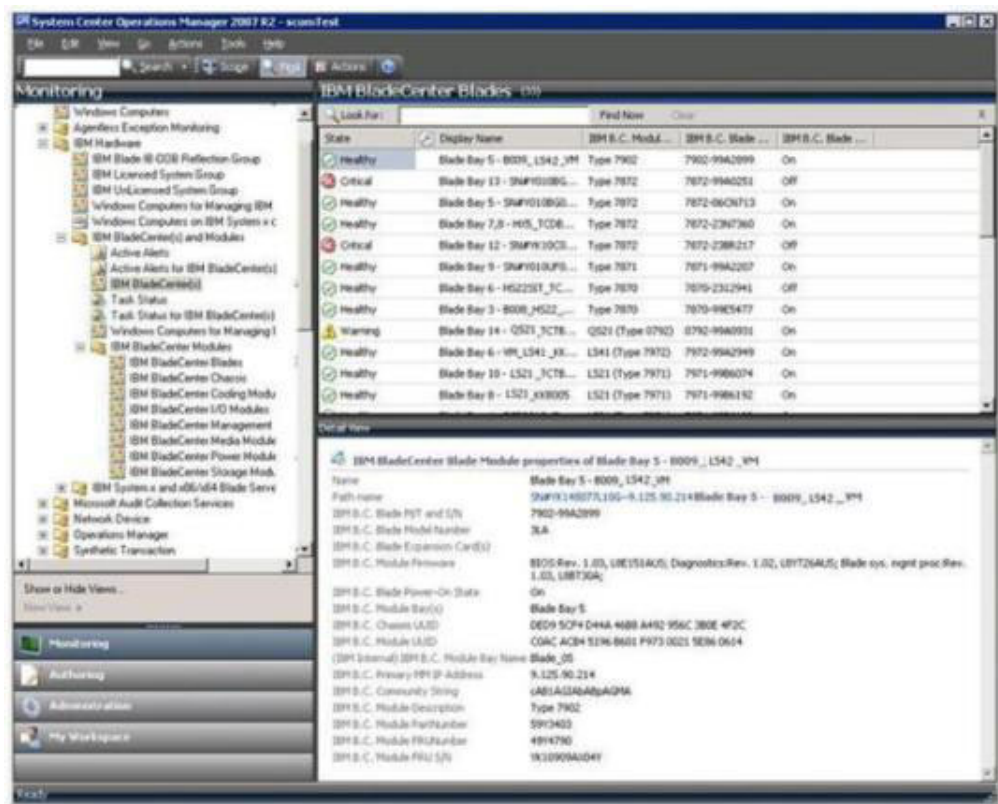


Figure 34. IBM BladeCenter Modules

- Click the **IBM System x and x86/x64 Blade Servers** view to display the views in the folder.

After discovering an IBM system with Windows, the IBM Hardware Management Pack classifies the system according to its system type and then adds the system to the view of **All IBM System x and x86/x64 Blade Servers** and to one of the following system group views, according to the system platform type:

- Active Alerts for IBM Software for HW Mgmt
- All IBM System x<sup>®</sup> and x86/x64 Blade Servers
- IBM Flex System x86/x64 Compute Nodes
- IBM System x Enterprise/Scalable Systems
- IBM System x iDataPlex Systems
- IBM System x Rack-mount Systems
- IBM System x Tower Systems
- IBM x86/x64 Blade Systems
- IBM Blade OOB-IB Reflection Group: This view provides the status of Windows computers on IBM x86/x64 Blade servers and the relationship between an IBM BladeCenter x86/x64 Blade server in the **IBM System x and BladeCenter x86/x64 Blade Servers** (monitored through Inband) and **BladeCenter(s) and Modules** (monitored through Out of band) folders.

**Note:** This view is available only when the premium features are enabled.

- Task Status
  - Unclassified IBM System x and BladeCenter x86/x64 Blade Systems (systems that are either too old or too new to be classified correctly)
  - Hardware Components of IBM System x or x86/x64 Blade Servers (folder)
- Click the **All IBM System x and x86/x64 Blade Servers** view to display the dashboard views of its systems and hardware components.

Each view within the **All IBM Systems x and x86/x64 Blade Servers** view provides a dashboard of health states and manageable hardware components for each system, as shown in the following figure.

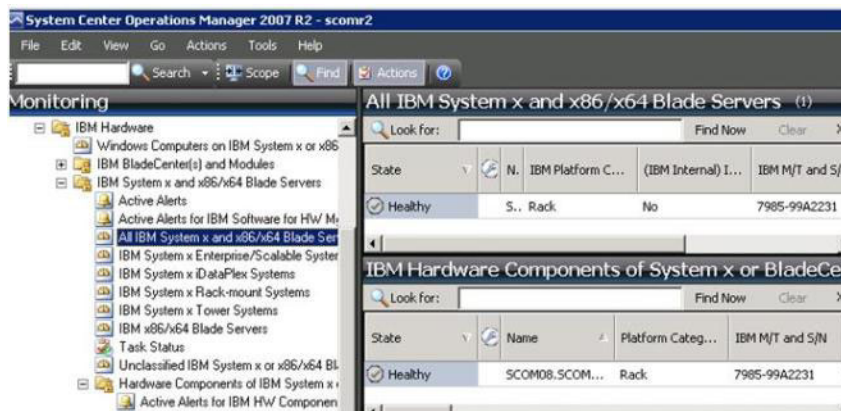


Figure 35. Dashboard view

---

## Adding an IBM system that will be managed by the Operations Manager

Use the Microsoft Operations Manager 2007 Discovery Wizard to discover and add IBM systems that will be managed by the Operations Manager. The Discovery Wizard deploys the IBM Hardware Management Pack to the discovered system.

**Note:** The Discovery Wizard does not show systems that are already being monitored.

### Optional steps before starting this task

When the IBM License Entitlement Pack is installed and the Root Management Server of Microsoft System Center Operations Manager is registered with the IBM License Entitlement Pack, the Hardware Management Software Configuration Advisor for IBM Systems (SW Configuration Advisor) program analyzes the software dependencies of the IBM Hardware Management Pack for Windows computers managed by Microsoft System Center Operations Manager.

For details about the IBM License Entitlement Pack, contact your IBM sales representative.

### How to check software dependencies on the remote computer

The following procedure describes how to check for software dependencies by using the Software Configuration Advisor program.

#### Procedure

1. Log in to the Operations Manager server and open a command shell window, a DOS commands window, or a PowerShell command window.
2. Change the directory to the toolbox directory. By default, the toolbox directory path is: %ProgramFiles%\IBM\IBM Hardware Management Pack\toolbox. (This directory is located after the installation directory of the IBM Hardware Management Pack for Microsoft System Center Operations Manager).
3. Start `ibmSwConfigurationAdvisor.vbs`. This is the program name of the Hardware Management Software Configuration Advisor for IBM Systems. You can use the following options when running this program:

**/help:**

Provides the syntax of the `ibmSwConfigurationAdvisor.vbs` program.

**/opt detail:**

Provides additional detail information about the targeting computer.

4. Enter the following required account information for the account that is a member of the Administrators role for the Windows computer.

This program is in the format of a Microsoft Visual Basic Script.

- Computer Name: `IBMUIM004`
- Domain name: `d205`
- Username: `admin@d205`
- Password: `aWd25$tg`

The target computer information is listed in the program's Analysis Summary:

```

> cscript //nologo cscript //nologo ibmSwConfigurationAdvisor.vbs
/remote IBMUI004 d205 admin@d205 a@d25tg
=====>> Computer: IBMUI004 <<=====
----- Analysis Summary -----
Computer Name       : IBMUI004
Manufacturer        : IBM                               MT-Model-S/N: 7870-AC1-
0XX493
Machine Summary    : BladeCenter HS22 -[7870AC1]-
-- Operating System --
Detected : Microsoft Windows Server 2008 R2 Enterprise (64-bit) - No
Service Pack Information
-- SMBIOS IPMI Support --
Detected : Default System BIOS
SMBIOS IPMI Support is installed
-- MS IPMI --
Detected : Microsoft Generic IPMI Compliant Device
Microsoft IPMI Driver is running
-- Systems Director --
Detected : 6.2.1 (Director Platform Agent)
Systems Director is running
-- ServeRAID-MR,MegaRAID,ServeRAID-BR/IR,Integrated RAID --
Detected : ServeRAID-BR10i1

```

Figure 36. Hardware Management Software Configuration Advisor for IBM Systems program

5. Check the Hardware Management Software Configuration Advisor for IBM Systems report. This report provides a summary of the analysis results. If there are any software dependency problems reported, examine the report body for possible resolutions for the software dependencies.

**Example**

In many cases, multiple computers are the target of the software dependency analysis. Using a command shell pipeline increases the productivity of this analysis.

The following example for uses PowerShell to pipe a net view computer name list to ibmSwConfigurationAdvisor.vbs and save the program output in the file called "OneShotServey4IbmHwMp.txt".

```

PS C:\Program Files\IBM\IBM Hardware Management Pack\toolbox>
net view | where {$_.-match "\\") | % { $_.substring(2,21) } | %{
$_trim(1," ") } | % { cscript //nologo ibmSwConfigurationAdvisor.vbs
/remote $_ d205 admin@d205 a@d25tg >> OneShotServey4IbmHwMp.txt }

```

Figure 37. PowerShell example of net view

The sample shown in the figure above is dependent on the Windows network set up and PowerShell environment. Adjustments for the network configuration and the PowerShell installation may be required.

## Using the Discovery Wizard to add an IBM system

The following procedure describes how to add an IBM system that will be managed by the Operations Manager.

### Before you begin

Log in to the Operations Manager server as Administrator to complete this task.

### Procedure

1. Click **Administration > Device Management > Agent Managed > Discovery Wizard** to start the Computers and Device Management Wizard. From the **Actions** menu, you can also select **Configure computers and**

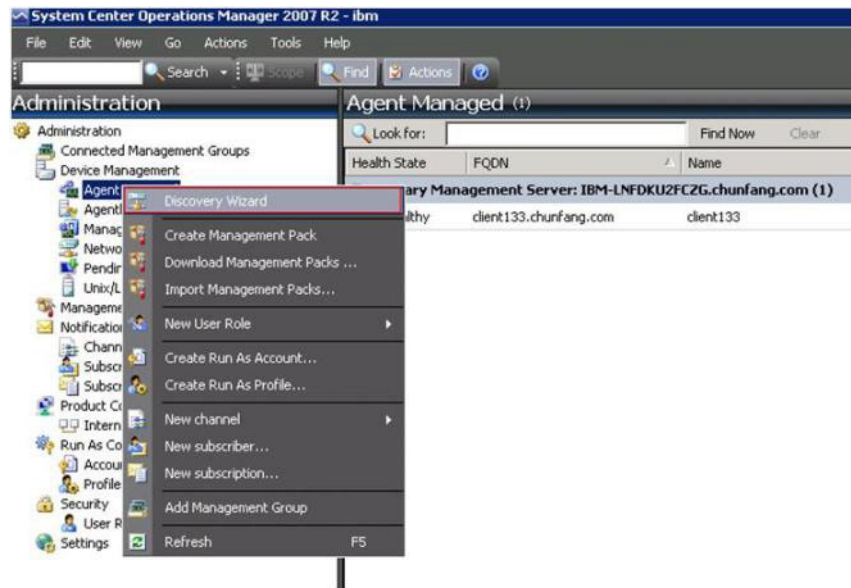


Figure 38. Using the context menu to select the Discovery Wizard

devices to manage.

**Note:** For Microsoft System Center Operations Manager 2007 SP1, the interface is somewhat different, as shown in the following figure.

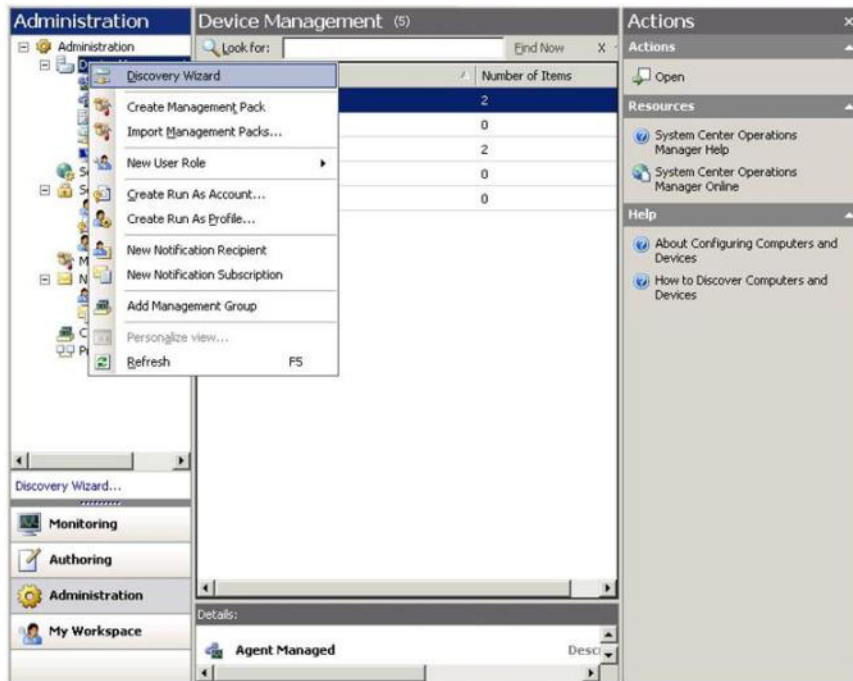


Figure 39. Using the context menu to select the Discovery Wizard (SP1)

2. Click Next if the Introduction page opens.

**Note:** The Introduction page does not display if the Computer and Device Management Wizard has been run before and you selected **Do not show this page again**. If you would prefer that the introduction page not be displayed again, select the **Do not show this page again** check box, before clicking **Next**.

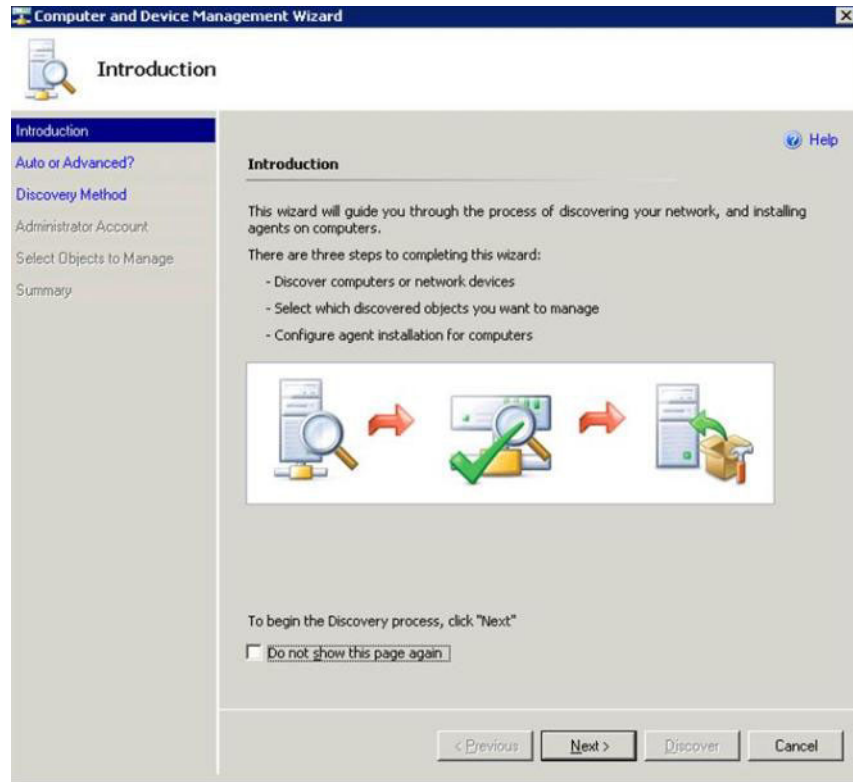


Figure 40. Computer and Device Manager Introduction

3. Select **Advanced discovery** on the Auto or Advanced page.

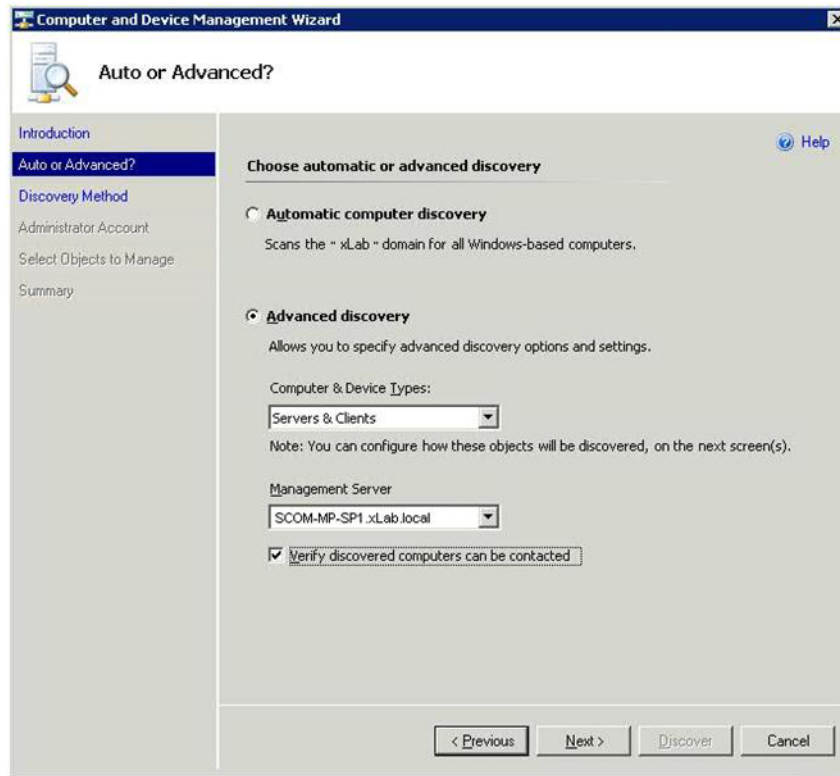


Figure 41. Selecting Auto or Advanced Discovery Method

4. From the **Computer & Device Types** list, select **Servers & Clients**.
5. From the **Management Server** list, select the **Management Server** to be used for discovery.
6. Select the **Verify discovered computers can be contacted** check box.
7. Click **Next** to open the Discovery Method page.



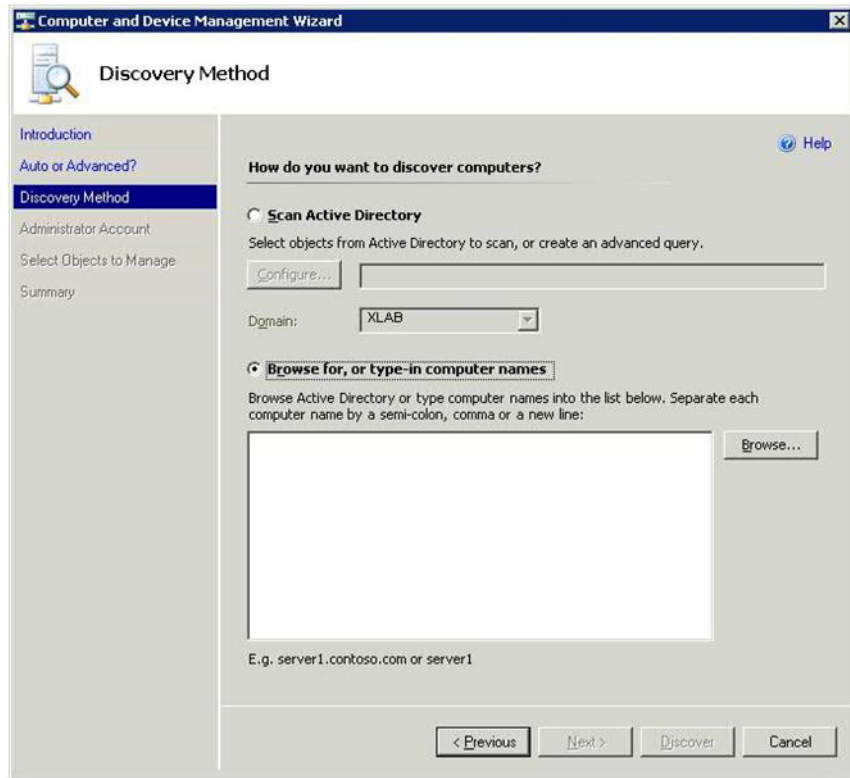


Figure 42. Discovery Method

8. Click **Browse for, or type-in computer names**, then click **Browse** to locate the computer name or enter the computer name of the IBM system and click **Next**.

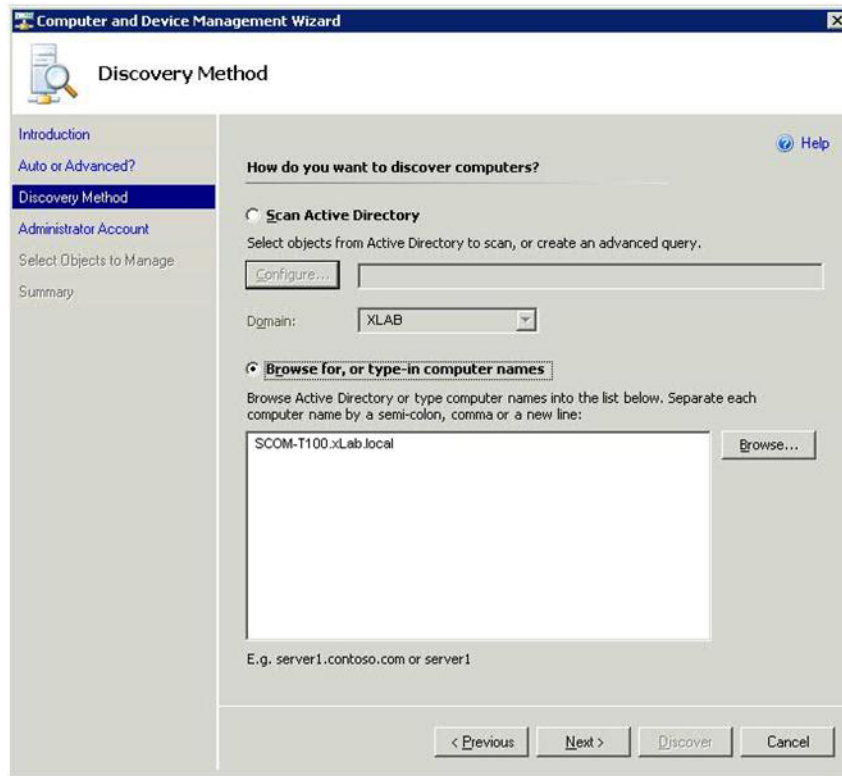


Figure 43. Discovery Method with sample information

9. On the Administrator Account page, choose one of the following options:
  - Click **Use selected Management Server Action Account** and then click **Next**.
  - Click **Other user account** and enter the following information:
    - User Name
    - Password
    - Domain Name of an account that is a member of the Administrator role
10. Click **Discover** to open the Discovery Progress page.

**Attention:** The time it takes for the discovery process to finish depends on the number of computers in the network and other factors. The Discovery Wizard might return up to 4,000 computers if you selected the **Verify discovered computers can be contacted** check box, or up to 10,000 computers if the check box is not selected.

When the discovery is finished, the Discovery Results are displayed and you can select the objects to manage.

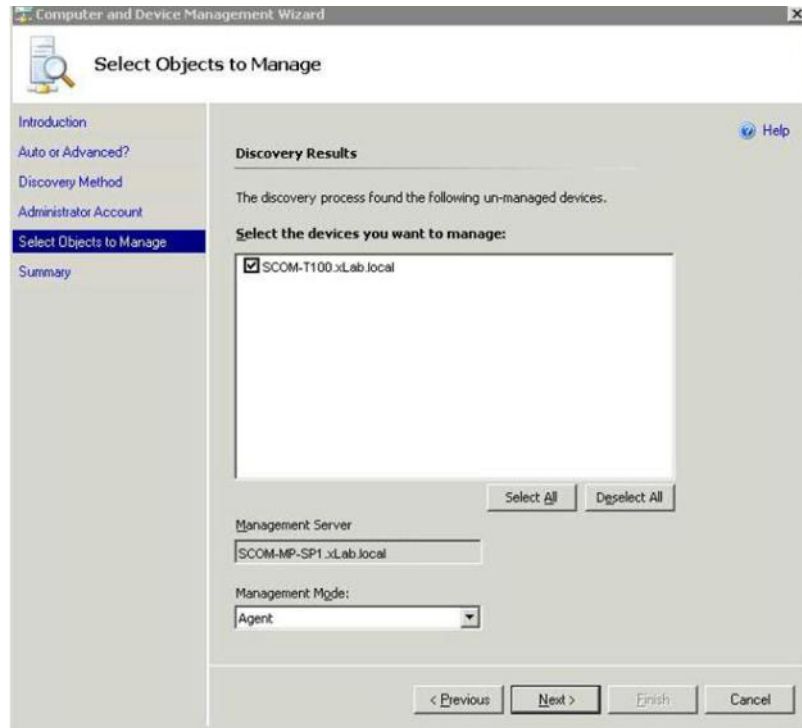


Figure 44. Select Objects to Manage

11. From the **Select the devices you want to manage** list, select the devices to be managed by selecting an individual device or by clicking **Select All**. You also have the option of clicking **Deselect All** to change the devices you want to manage.
12. From the **Management Mode** list, select **Agent** and click **Next**.

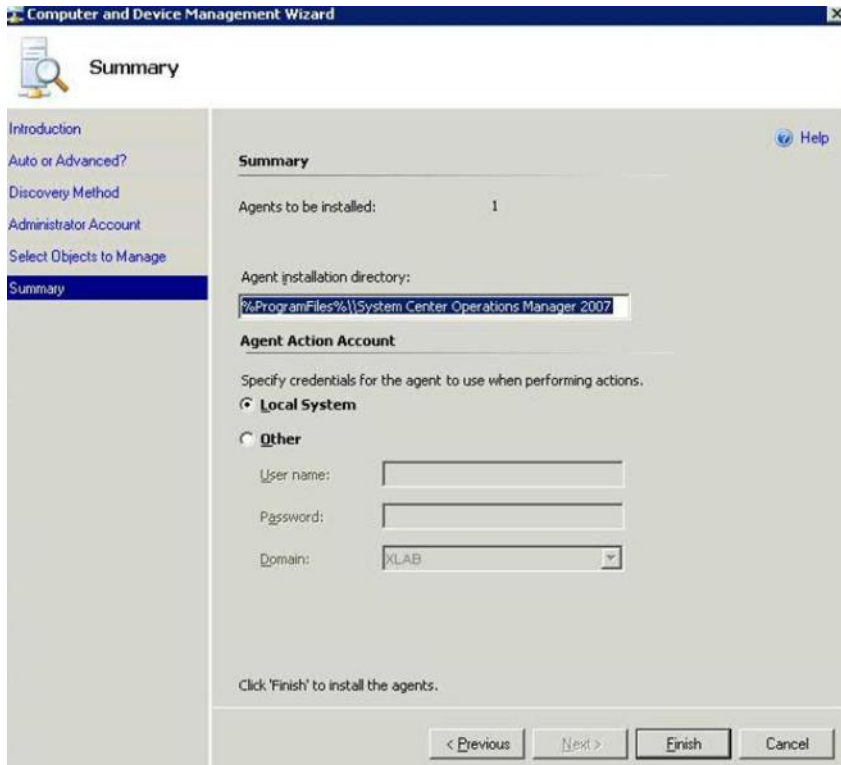


Figure 45. Computer and Device Management Wizard Summary

13. On the Summary page, click **Finish**. The Agent Management Task Status page is displayed.

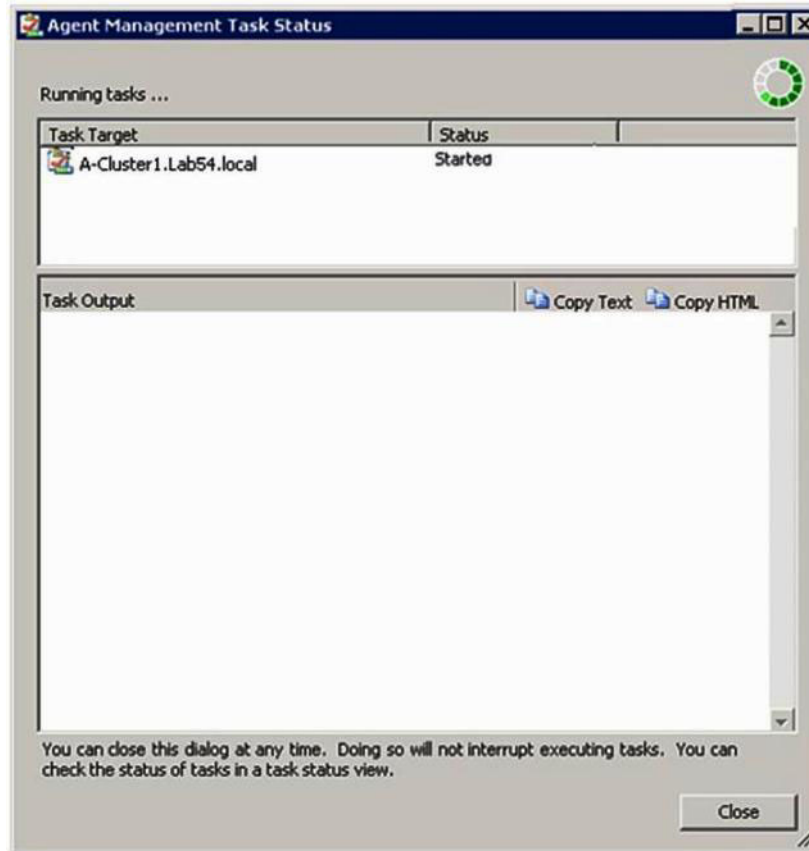


Figure 46. Agent Management Task Status

- To view the agent installation task status, review the Agent Management Task Status page.

**Note:** While this task is running, an indicator is displayed on the upper right side of the page. You can close this page at any time without interrupting the task.

- Optional: To check the Agent Management Task Status and verify that the status of selected computers, changed from *Queued* to *Success*, click **Monitoring > Task Status**.
- Click **Close** on the Agent Management Task Status page.

## What to do next

For more information about using the Discovery Wizard, see Technet: Systems Center Technical Resources.

---

## Viewing inventory

The following procedure describes how you can use the Microsoft System Center Operations Manager to view a complete inventory of configured management modules.

### Procedure

1. To view IBM BladeCenters and their modules, in the Microsoft System Center Operations Manager Console window, within the Computer and Groups pane, click **Computers and Groups View > IBM Hardware > IBM BladeCenters and Modules**
2. To view the IBM System x servers, BladeCenter blade servers, and other individual systems that have been discovered, click **Computers and Groups View > IBM Hardware > IBM System x and x86/x64 Blade Servers** .

---

## Monitoring the health of systems, hardware components, and other targets

The IBM Hardware Management Pack discovers and monitors the health of the following hardware components: fans, memory, management controllers, network adapters, power supplies, processors, storage, temperature sensors, and voltage sensors. The IBM Hardware Management Pack can also discover and monitor the health of system-management software, such as IBM Systems Director Agent, Intelligent Platform Management Interface (IPMI) driver, IBM IPMI Mapping Layer, and ServeRAID™ Manager Level 1 Agent.

### Before you begin

Log in to the Microsoft System Center Operations Manager operations console.

### About this task

Component discovery and health monitoring is dependent on firmware support, hardware compatibility, and management-software support. Because of these factors, not all components are discoverable. If a component is not discovered, it cannot be monitored or managed.

### Procedure

1. In the navigation pane, click **Monitoring > IBM Hardware** to display the folders and views that the IBM Hardware Management Pack adds to the Operations Manager Console.

2. Select either **IBM BladeCenter(s) and Modules** or **IBM System x and x86/x64 Blade Servers**.
3. Click **Active Alerts** to see if any Critical or Warning alerts are associated with your IBM hardware. The following figure shows an example of how Active Alerts might be displayed:

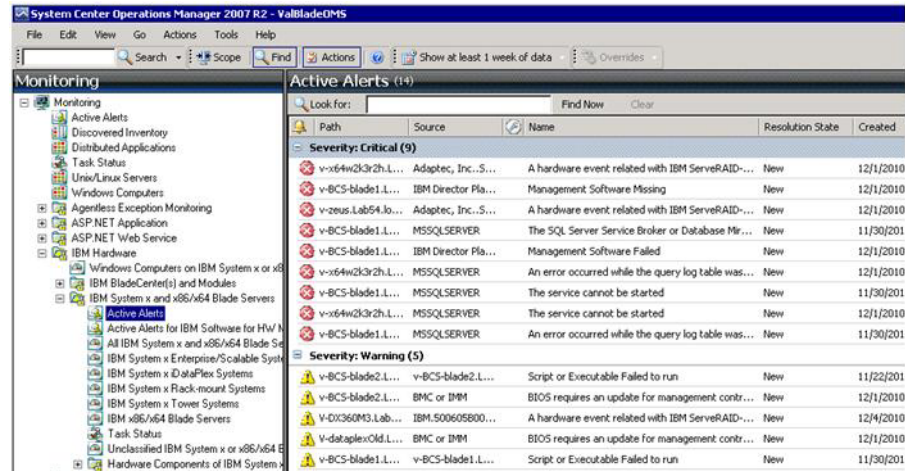


Figure 47. Active Alerts example

4. You can check the health of your systems, by using one or more of the following options:

**Windows Computer on IBM System x or x86/x64 Blade Servers:**

Provides the status of the Windows platform on each system in the IBM Hardware folder.

**IBM BladeCenter(s) and Modules:**

Provides a view of the health information for all modules. Select this view to check the status of all IBM BladeCenter chassis, and then select the **IBM BladeCenter Modules** view.

**IBM System x and x86/x64 Blade Servers:**

Checks the hardware status of all IBM systems.

**All IBM System x and x86/x64 Blade Servers:**

Lists the health indicators in the first column of the system dashboard, and the first column of the hardware components dashboard.

To check the status of a system in this view, select a group view.

## What to do next

For more information on how to use the Health Explorer for analyzing a critical problem, see “Using Health Explorer to identify and resolve problems” on page 75.

---

## Viewing alerts

The following procedure provides an example and instructions for using Microsoft System Center Operations Manager to view alerts sent from properly configured management modules and IBM System x systems and BladeCenter Blade servers.

### About this task

This task is performed from the Operations Manager Console.

### Procedure

- To view BladeCenter chassis alerts, click **Monitoring > IBM Hardware > IBM BladeCenters and Modules > Active Alerts**.

In **IBM BladeCenters and Modules** view, you can see the following components under each chassis.

- IBM BladeCenter Blades
- IBM BladeCenter Chassis
- IBM BladeCenter Cooling Modules
- IBM BladeCenter I/O Modules
- IBM BladeCenter Management Modules
- IBM BladeCenter Media Modules
- IBM BladeCenter Power Modules
- BladeCenter Storage Modules

An alert from the BladeCenter creates an additional alert for IBM x86/x64 Blade servers that may be affected by this alert condition, when the Windows Operating system is installed on an IBM x86/x64 Blade server and when the premium feature is enabled.

The **IBM Blade OOB-IB Reflection** group view shows the health of IBM x86/x64 Blade Server based on this additional alert from IBM BladeCenters and Modules.

- To view individual System x, xSeries, BladeCenter blade server, and other systems, click **Monitoring > IBM Hardware > IBM System x and x86/x64 Blade Servers > Active Alerts**.

The IBM x86/x64 Blade alert reflecting BladeCenter chassis alerts is displayed in this **Active Alerts** view, when the Windows Operating system is installed on IBM x86/x64 Blade Server and when the premium feature is enabled.

The IBM x86/x64 Blade alert displaying BladeCenter chassis alerts contains information about the malfunctioning component location in IBM BladeCenter.



- To review the details of the malfunctioning component, click **Monitoring > IBM Hardware > IBM BladeCenters and Modules > Active Alerts** to see the **Active Alerts** view for BladeCenter chassis alerts.

**Notes:**

- The IBM Hardware Management Pack has limited support for tools like WinEvent.exe that generate IBM Systems Director events and do not fully prescribe specific target instances.
- In some circumstances, the WinEvent.exe tool does not correctly support the **event ID** and the **event description**. This can cause the WinEvent.exe tool to be unreliable for displaying all events.
- All WinEvents are reported under one monitor.
- Successfully simulated events are displayed in the Operations Manager Console under the **Alerts** view and the **Events** view.
- Monitored systems that have IBM Systems Director Agent 5.1.x installed and that use the WinEvent.exe tool can cause errors to reoccur even after you manually clear the alerts from the Health Explorer view.
- To eliminate such an event recurrence, delete the IBM\director\cimom\data\health.dat file and all IBM\director\cimom\data\health.dat\\*.evt files from the client system and restart the system.
- To open a monitoring view, right-click a BladeCenter chassis, a System x server, a BladeCenter Blade server, or any other system. You can monitor these systems by using: the **Alerts** View, the **Diagram** View, the **Event** View, and the **State** View.

## Locating and viewing hardware errors

You can locate and view hardware errors by navigating to **All IBM System x and x86/x64 Blade Servers**.

---

## Using Health Explorer to identify and resolve problems

The following procedure describes how you can use Health Explorer to identify and resolve error states that occur when monitoring IBM systems and hardware components.

### About this task

To perform a quick check of existing alerts on your IBM hardware, select one of the following views:

- Active Alerts
- Windows Computers on IBM System x or x86/x64 Blade Servers
- All IBM System x and x86/x64 Blade Servers

Health Explorer can assist you in troubleshooting alerts. Use Health Explorer to view, learn about, and take action on alerts, state changes, and other issues raised by a monitored object.

For example, if you see a critical error when you are monitoring your systems and hardware components, as shown in the figure below, use the following procedure to identify and resolve the error.

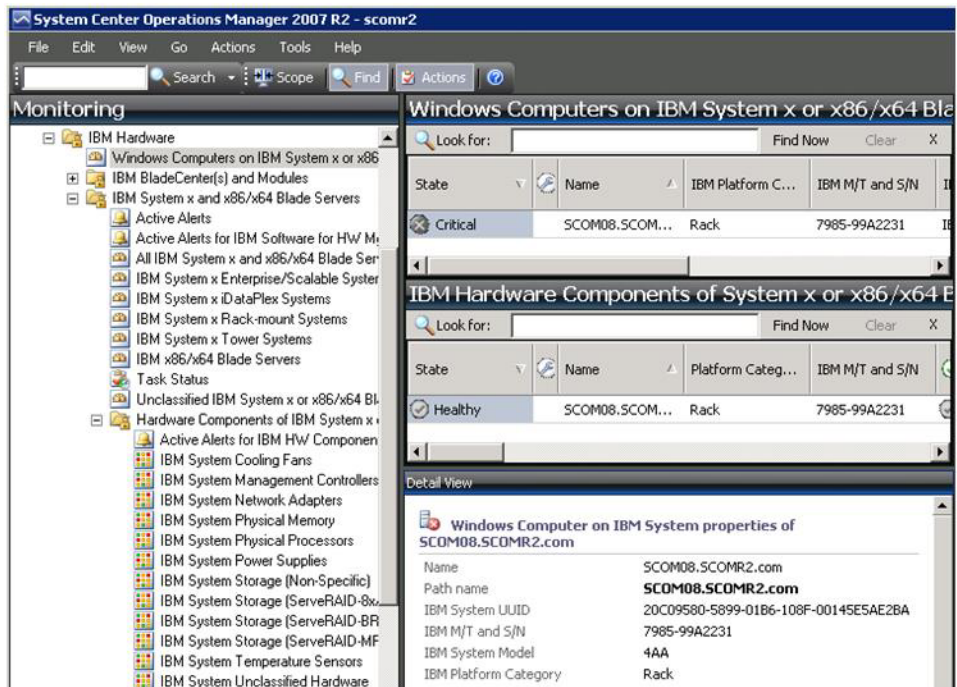


Figure 48. Example of a critical error showing up in a managed system

## Procedure

1. When there is a warning or critical alert, open Health Explorer by selecting **All IBM System x and x86/x64 Blade Servers**, and then double-click **state**.

**Note:** By default, Health Explorer opens with all failed monitors that are displayed in an expanded view.

The following figure shows how such an error might be displayed in the Health Explorer:

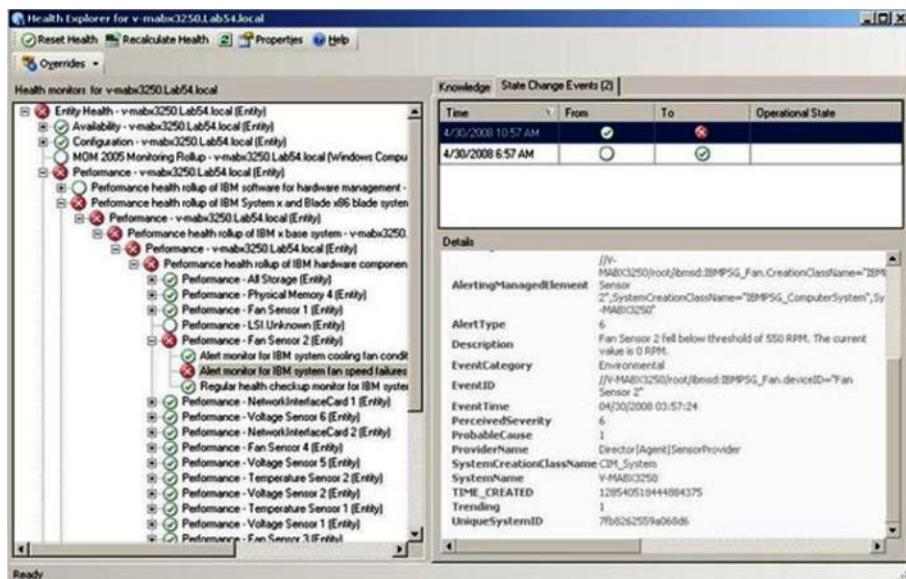


Figure 49. Example of hardware components causing a system to be in error

2. If there are no warnings or critical alerts visible:
  - a. Select an IBM system in the **All IBM System x and x86/x64 Blade Servers** view.
  - b. Right-click the system to show its context menu.
  - c. Click **Open** and then click **Health Explorer** to view the **system\_name**.
3. Use Health Explorer to identify the basal-level health monitor indicating an error. This indication should refer to a particular component instance. As shown in the figure above, the cause of the error is a faulty fan.
4. Click **State Change Events** in the results pane for details about the latest state change event.

The date and the time that the fan failed is displayed. You can also read details about the nature of the error. When the premium feature is enabled, the IBM BladeCenter Blade Out of Band Health Reflection Rollup reflects the component health in the BladeCenter.

5. Check the **IBM BladeCenters and Modules** folder view for further analysis when you see a warning or critical alert on IBM BladeCenter Blade Out of Band Health Reflection Rollup.

### What to do next

To learn more about how knowledge pages can assist you in resolving an error state and to learn more about hardware components, see “Using knowledge pages to resolve problems.”

---

## Using knowledge pages to resolve problems

Knowledge pages provide information about errors, events, and components. To learn more about your systems, hardware components, and how to resolve errors when they occur, refer to the knowledge pages.

### About this task

This figure shows an example of how an error might be displayed in the Health Explorer:

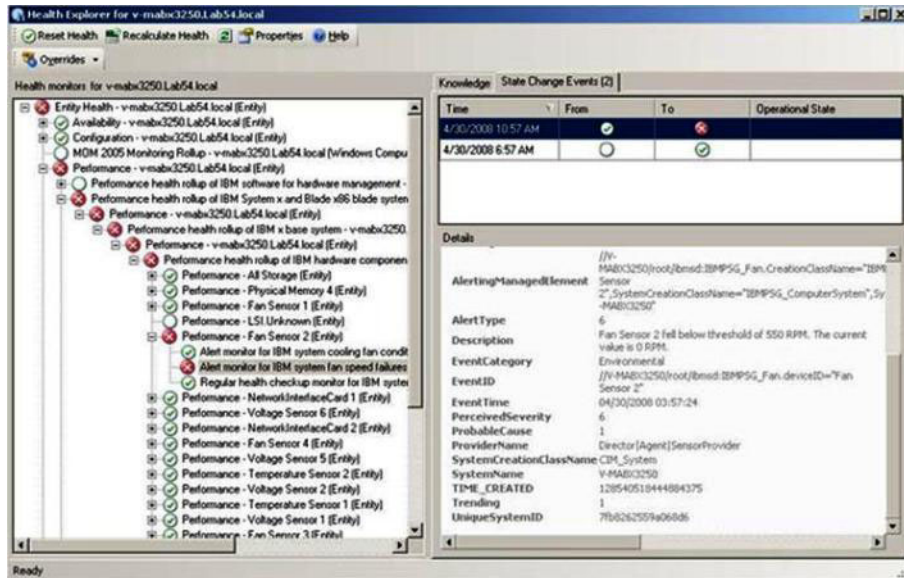


Figure 50. Example of hardware components causing a system to be in error

Knowledge pages are written by IBM developers and can help you understand more about IBM System x and x86/x64 Blade Servers events, alerts, components, and other information.

You can access the knowledge pages in these ways:

- Use the **Health Explorer/Monitors** view to access IBM Hardware Management Pack monitor information.
- Use the **Events** view to access information about the event.
- Use any links provided in the knowledge pages to access related hardware event information.

The following procedure describes how to use the knowledge pages in further detail.

## Procedure

1. Click **Knowledge** in the right pane of Health Explorer to read about the error event, including explanations and necessary steps that might help you to fix the problem.

Read the information in the **Knowledge** tab for the Alert monitor highlighted in the navigation pane to check whether a manual **Reset Health** is required, and for information about how to resolve the error if extra steps are needed.

This figure provides an example of how this page is displayed.

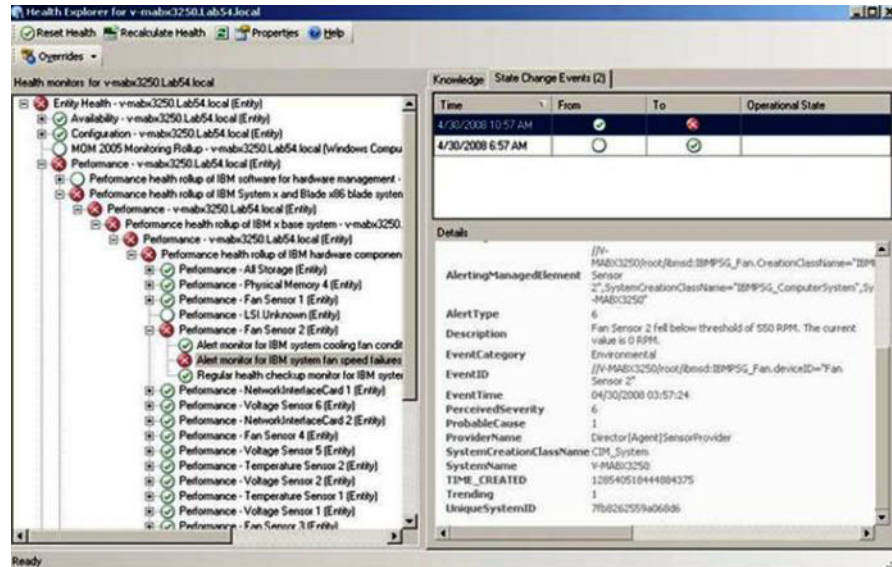


Figure 51. Example of a knowledge page that describes an error event

Some knowledge pages have links to another knowledge page for possible causes and suggested actions. These pages might describe specific errors and their remedies or describe hardware components.

2. Click the **Fan speed is outside the healthy range** link. The link opens another knowledge page, as shown in the figure below.

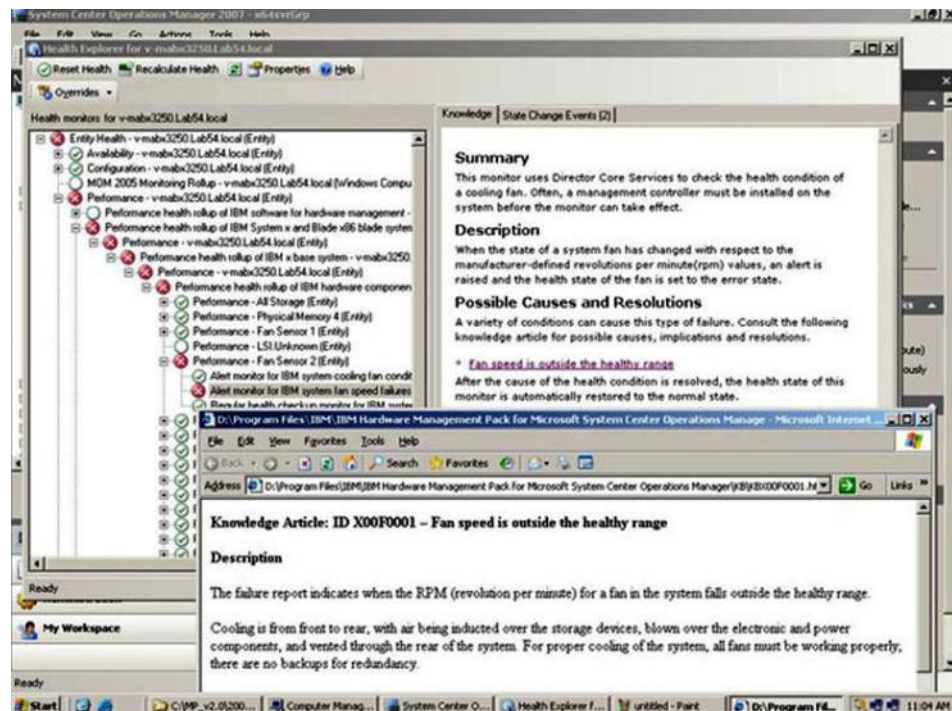


Figure 52. Example of one knowledge page linking to another

3. Perform the procedure identified in the knowledge pages to resolve the error and reset the health sensor, if necessary.

## What to do next

The knowledge pages are also accessible through the Active Alerts view.

To view the Alert Properties, double click an Alert. The Alert description is displayed in the **General** tab. The **Product Knowledge** tab includes a link to the knowledge page. The figure below provides an example of the Alert Properties window for an Alert.

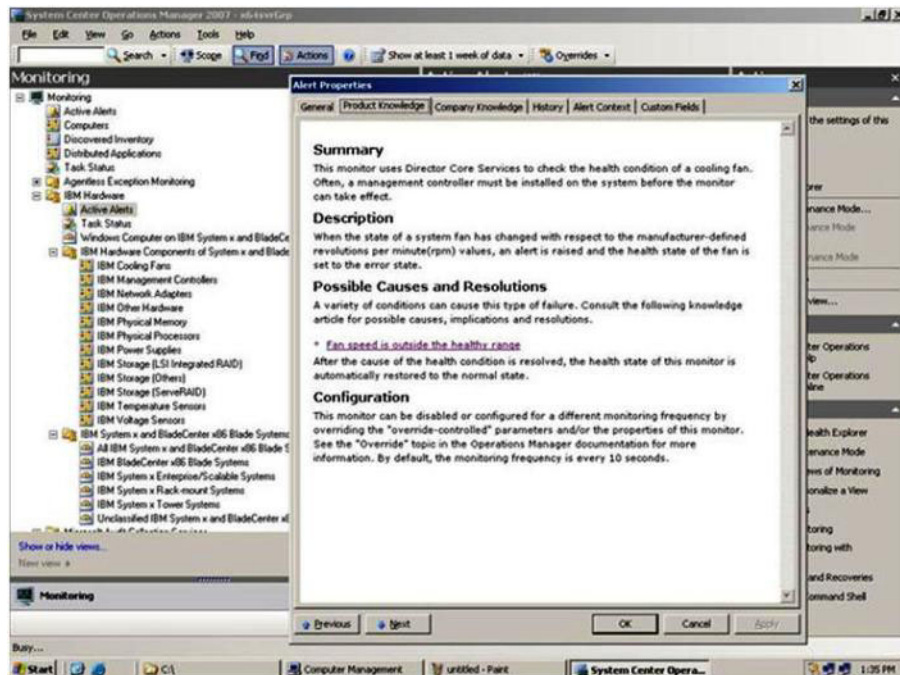


Figure 53. Example of Alert Properties

---

## Using premium features

This section describes how to use the premium features. The premium features are available when the IBM Hardware Management Pack installation is registered with the IBM Upward Integration for Microsoft System Center Installer.

For more information about the premium features, see "Premium features" on page 1.

## Remote power on and off of BladeCenter x86/x64 Blade servers

This feature allows you to remotely control the IBM BladeCenter Blade module and select power on, off, or shutdown of the operating system. When the premium feature is enabled, this task is available in the Actions pane of the Operations Manager Console.

### Remote shut down of an operating system

The following procedure provides instructions for an orderly shut down of an operating system on the IBM BladeCenter x86/x64 Blade module using the physical location of the Blade.

### About this task

This task is performed from the Operations Manager Console.

### Procedure

1. Click **Monitoring > IBM Hardware > IBM BladeCenter(s) and Modules > IBM BladeCenter Blades**.
2. From the **IBM BladeCenter Blades** view located in the results pane of the Operations Manager Console, select a **Blade server**.
3. In the Actions pane, select **IBM BladeCenter: Shutdown Operating System on this Blade**.

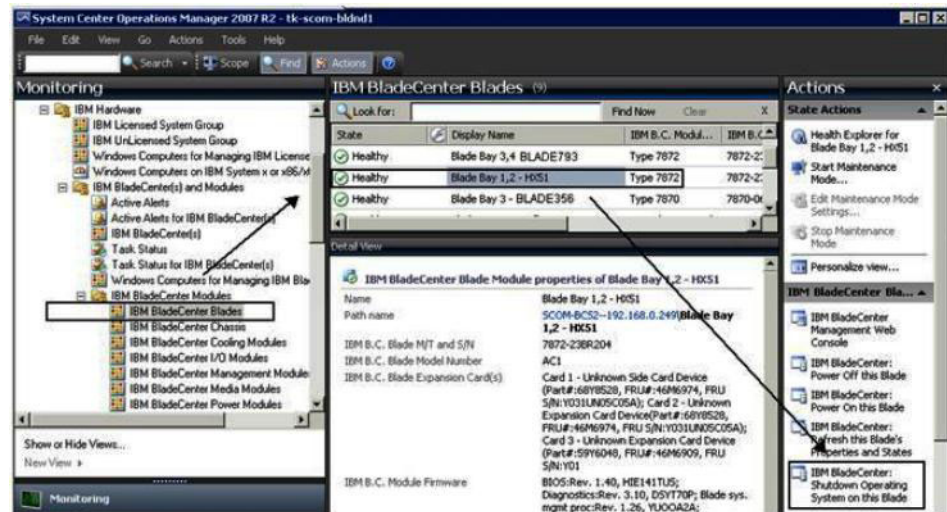


Figure 54. Operations Manager Console premium feature is enabled example

4. Verify the task targets by checking the (top-middle) results pane of the Operations Manager Console.



Figure 55. Task Status for Shutdown Operating System on this Blade

5. Click **Run**.





Figure 56. Task status indicating the shutdown task has been sent to this Blade

The task status window indicates that the task has been sent to the IBM BladeCenter for the target blade server.

6. Click **Close**.

When the premium feature is not enabled, the task fails. A message is displayed in the Task Output section indicating that the free version of the IBM Hardware Management Pack is being used.

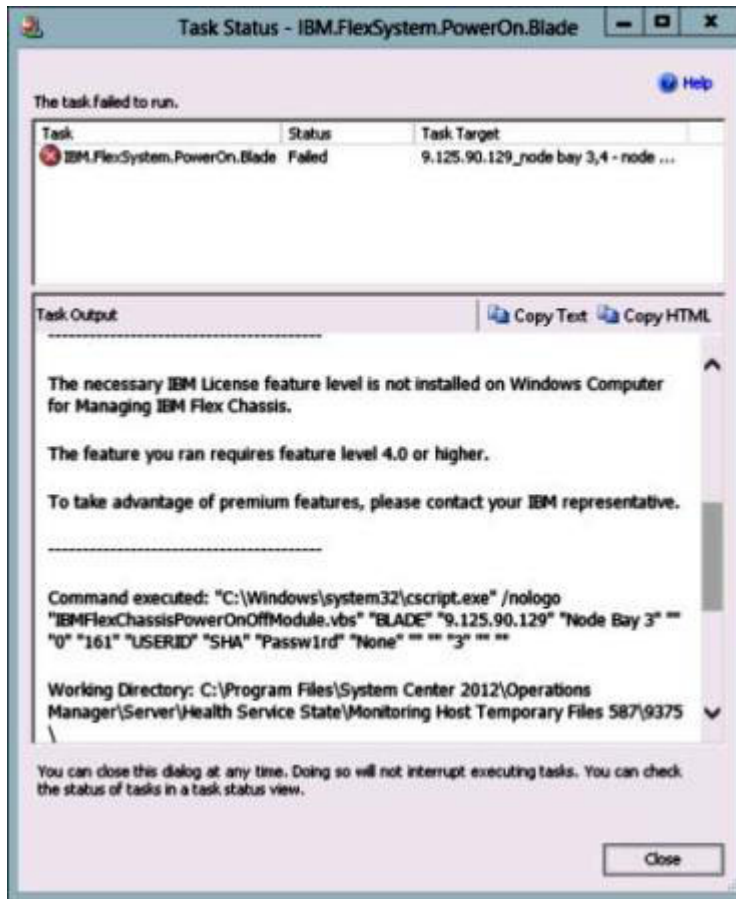


Figure 57. Example of a Task Output message

7. Click Close.
8. In the Actions pane, click **IBM BladeCenter: Refresh this Blade's Properties and Status** for an immediate Blade power status check.

### Remote Power On using the server name

The following procedure provides an example and instructions for the remote Power On feature by using the server name, IBM BladeCenter x86/x64 Blade .

## About this task

This task is performed from the Operations Manager Console.

## Procedure

1. Click **Monitoring > IBM Hardware > IBM System x and x86/x64 Blade Servers > IBM x86/x64 Blade Servers**.
2. Click a **Blade Server** in the IBM x86/x64 Blade Servers view located in the top middle pane of the Operations Manager Console.

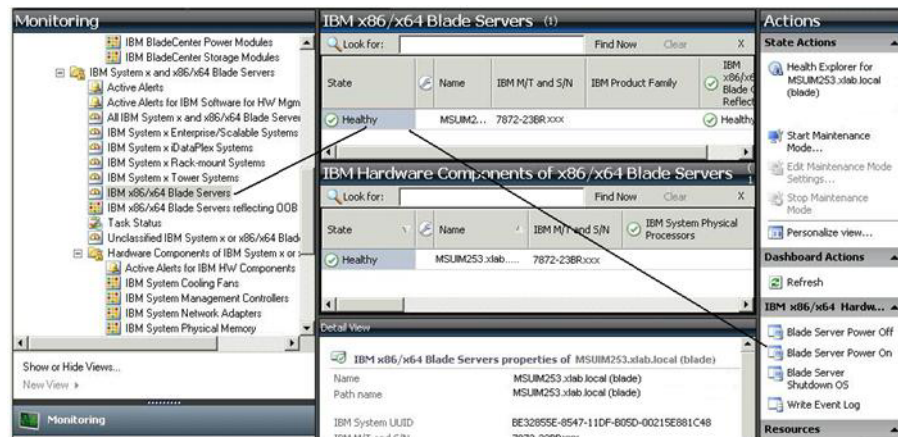


Figure 58. Example of Blade Server Power On task

3. In the Actions pane, select **Blade Server Power On**.

After the Blade Server Power On task has been started, a window opens and provides the task completion status. At the end of Task Output section, when the Power On task request has been sent to the BladeCenter, the <<--The task successfully completed. >> message is displayed.

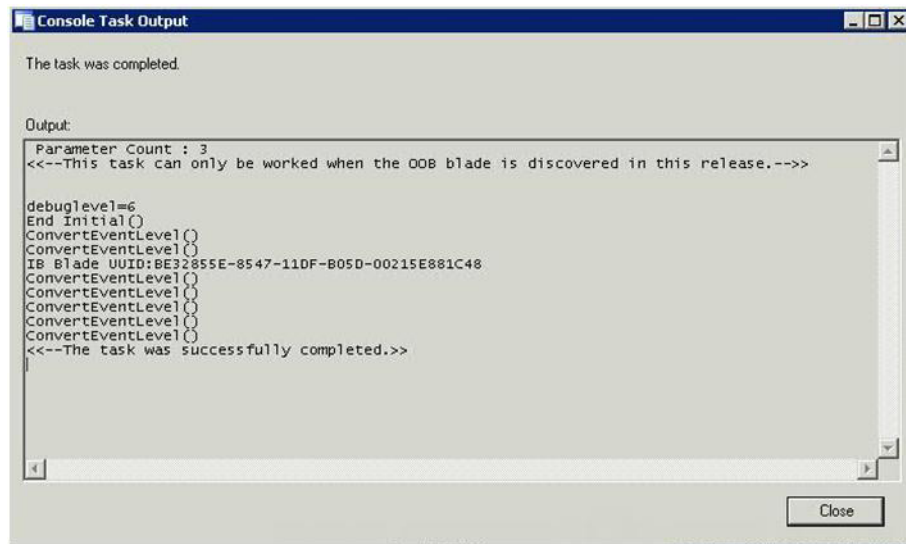


Figure 59. Task Output status for Power On task

4. Click **Close**.
5. In the Actions pane, select **IBM BladeCenter: Refresh this Blade's Properties and Status** for an immediate blade power status check.

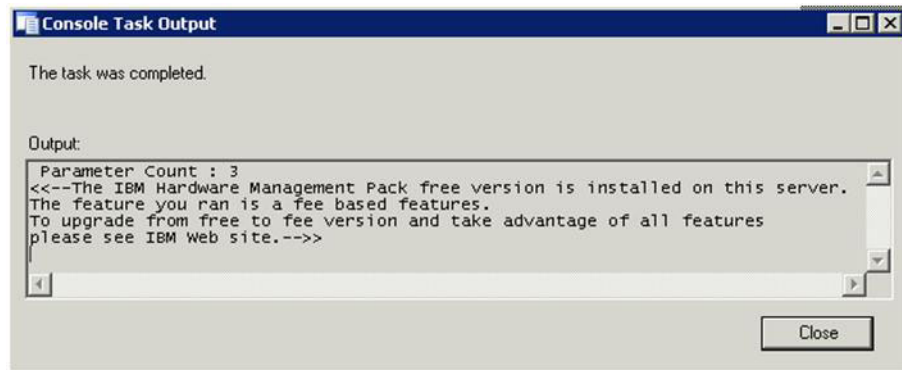


Figure 60. Task Output when premium feature is not enabled

6. Click **Close**.

## Setting the power threshold

IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 offers the ability to customize power consumption thresholds for Power Monitoring alerts. The following procedure provides instructions and an example of how to set and unset the power threshold.

### Before you begin

The target system must be capable of power monitoring to execute this task. This task is used to set or unset a warning or critical power threshold on a system. If you specify a blank or zero value for a particular threshold, that threshold is reset to its default value. Refer to the Detail View of this system under the **IBM Licensed Systems Group** to see the current threshold values and the *MonitoringCapable* property.

### About this task

This task is performed from the Operations Manager Console.

### Procedure

1. Click **Monitoring > IBM Hardware > IBM Licensed System Group**.
2. Click **Server** in the **IBM Licensed System Group** view located in the top middle pane.

3. Click **Set/Unset Power Threshold** in the right pane.

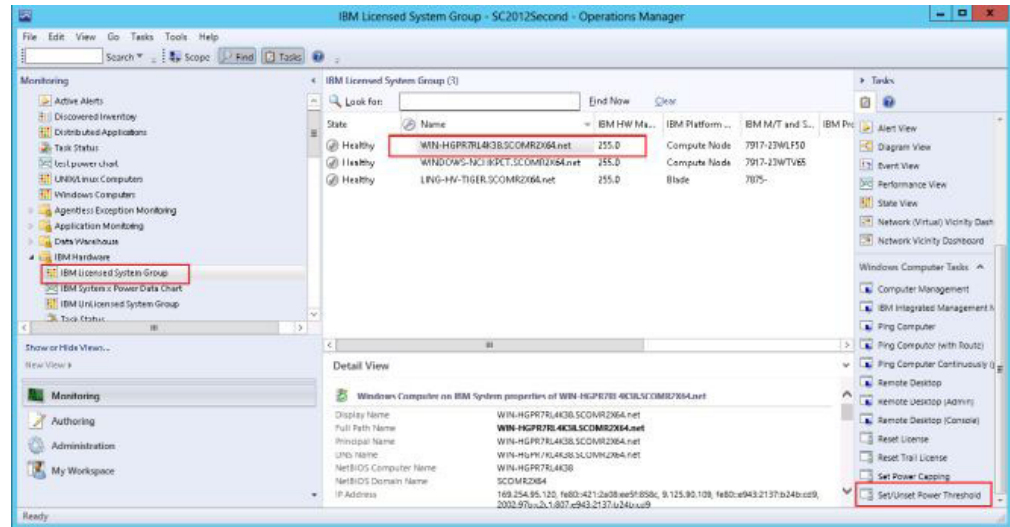


Figure 61. Example of Set/Unset Power Threshold task

4. Verify the task targets are located in the top pane of the Operations Manager Console.

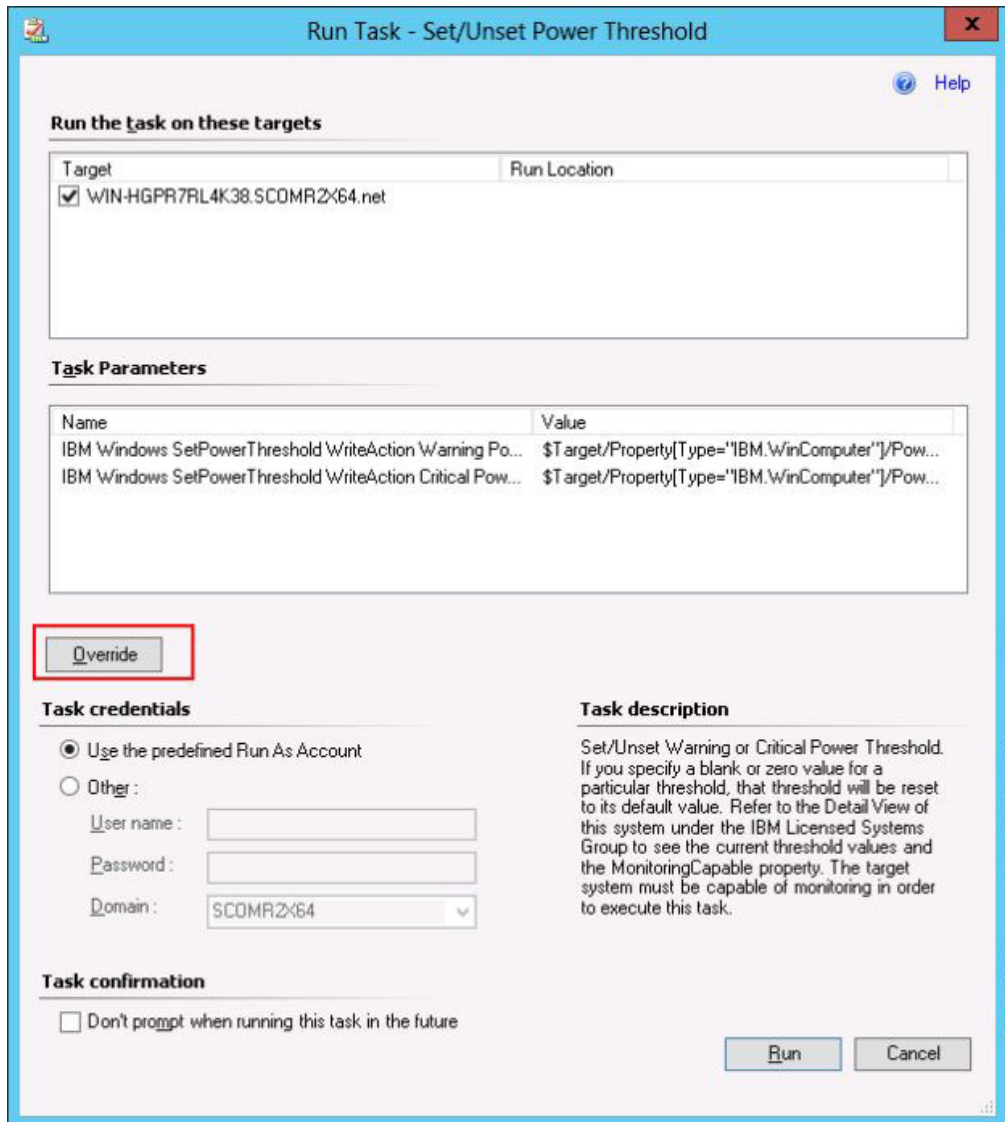


Figure 62. Target and task parameters of Set/Unset Power Threshold task

5. Click **Override** to override the power threshold values.

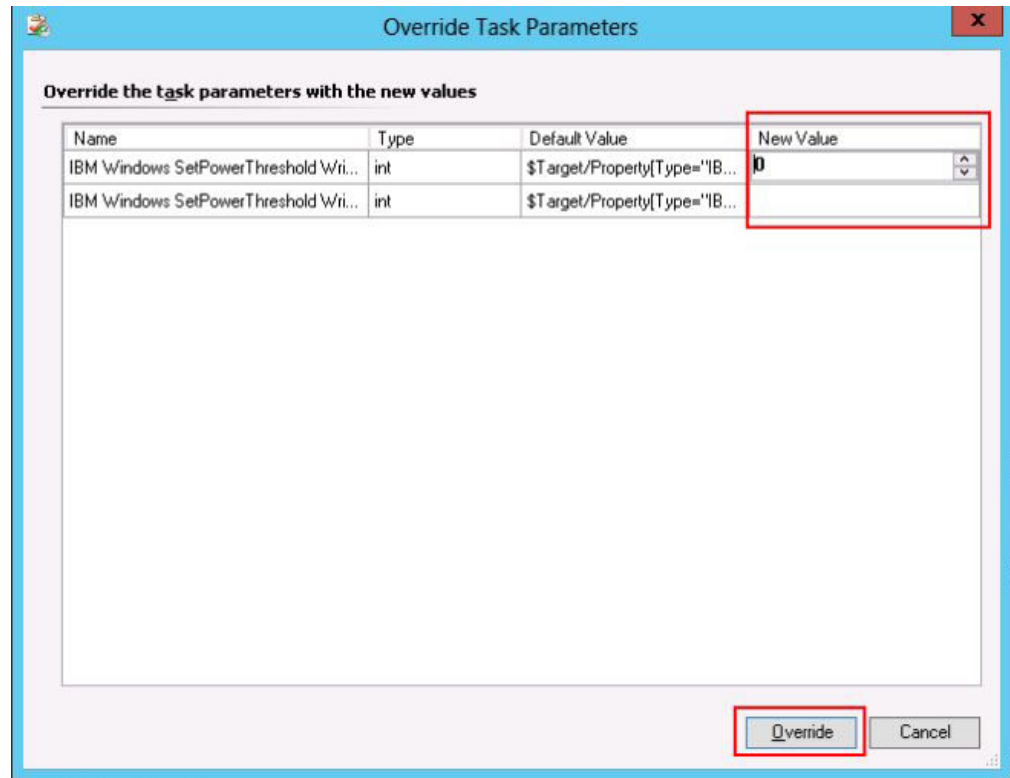


Figure 63. Override the task parameters of Set/Unset Power Threshold task

6. Enter new values for the threshold parameters and click **Override**.
7. Verify the values that you just set in the middle pane.

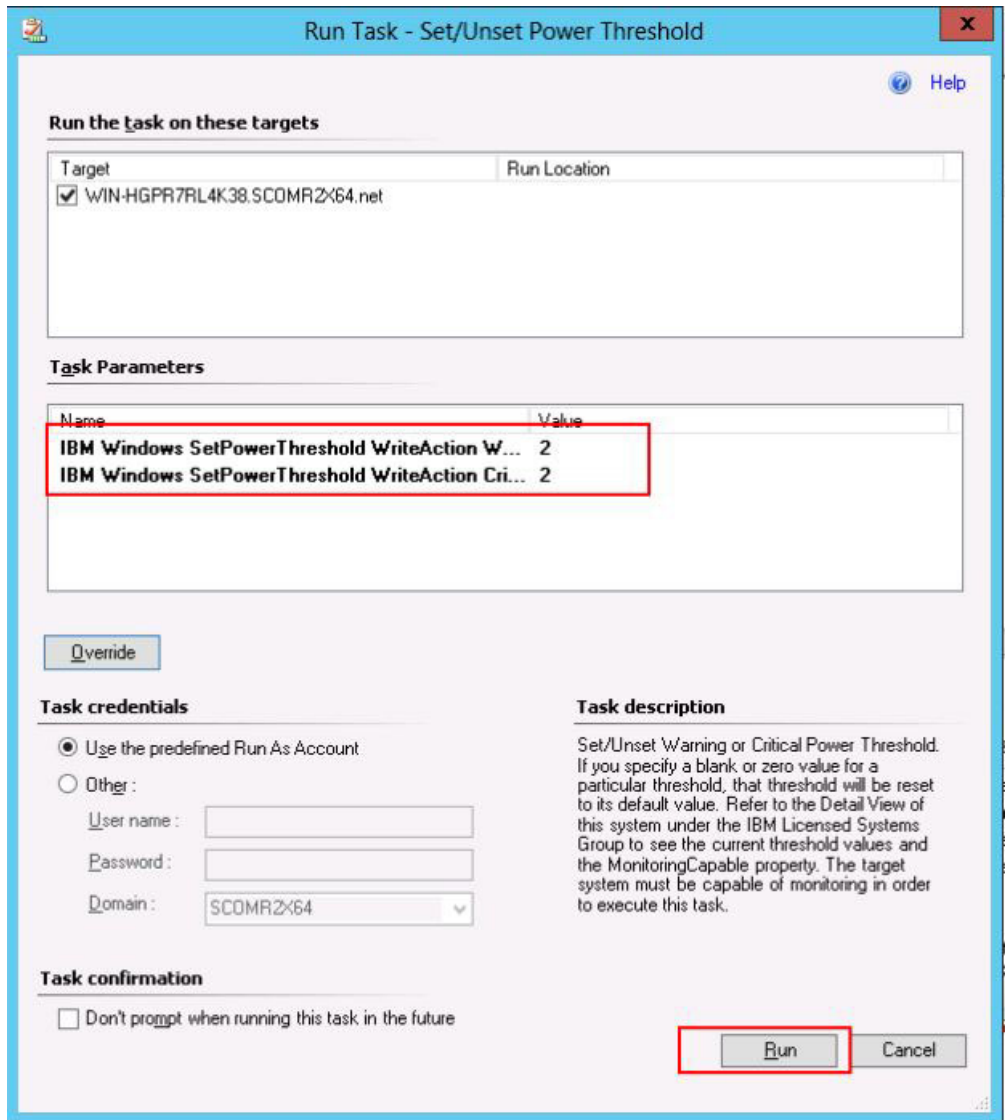


Figure 64. New values of the task parameters of Set/Unset Power Threshold task

8. Optional: Click **Override** if you want to change the values again.
9. After verifying the new values, click **Run**. The task status window indicates the task has been sent to the target server.



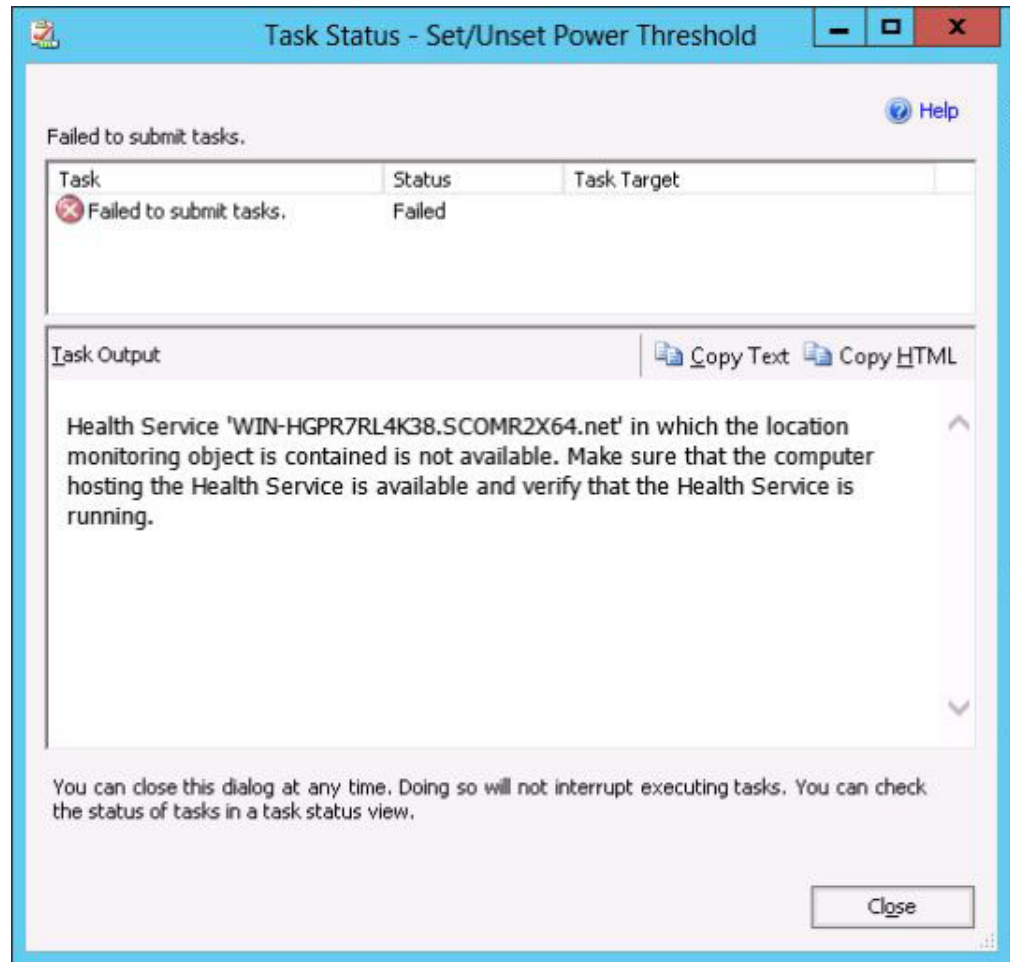


Figure 65. Task Status indicating the Set/Unset Power Threshold task has been sent to the target server

A message is displayed in the Task Output section indicating whether the task succeeded or failed.

10. Click **Close**.

## Enabling and setting power capping

IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 provides the ability to enable and set maximum power consumption wattage. The following procedure provides instructions and an example for setting power capping.

## Before you begin

Ensure that the target system is capable of power capping before starting this procedure. This task also requires the **User Access Control (UAC)** to be turned off on the target system. Refer to the Detail View of this system under the **IBM Licensed Systems Group** to see the current *CappingCapable*, *CappingEnabled*, *PowerMax*, *PowerMin*, and *PowerCap* values.

## About this task

This task is performed from the Operations Manager Console and is used to set or enable power capping on a system.

You must specify a value for the power cap in the **PowerMin** and **PowerMax** range.

## Procedure

1. Click **Monitoring > IBM Hardware > IBM Licensed System Group**.
2. Click **Server** in the **IBM Licensed System Group** view located in the top middle pane.
3. Click **Set Power Capping**.

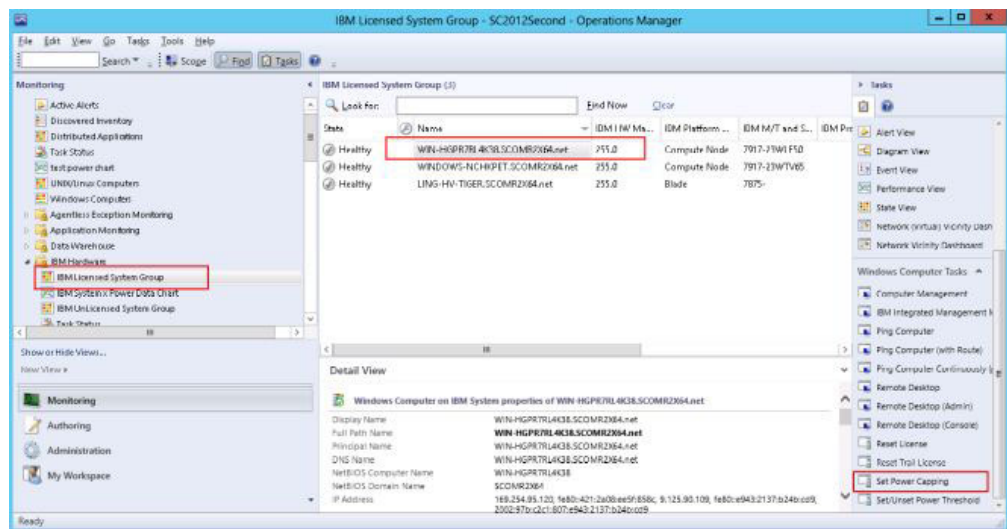


Figure 66. Example of Set Power Capping task

4. Verify the task targets are located in the top pane.

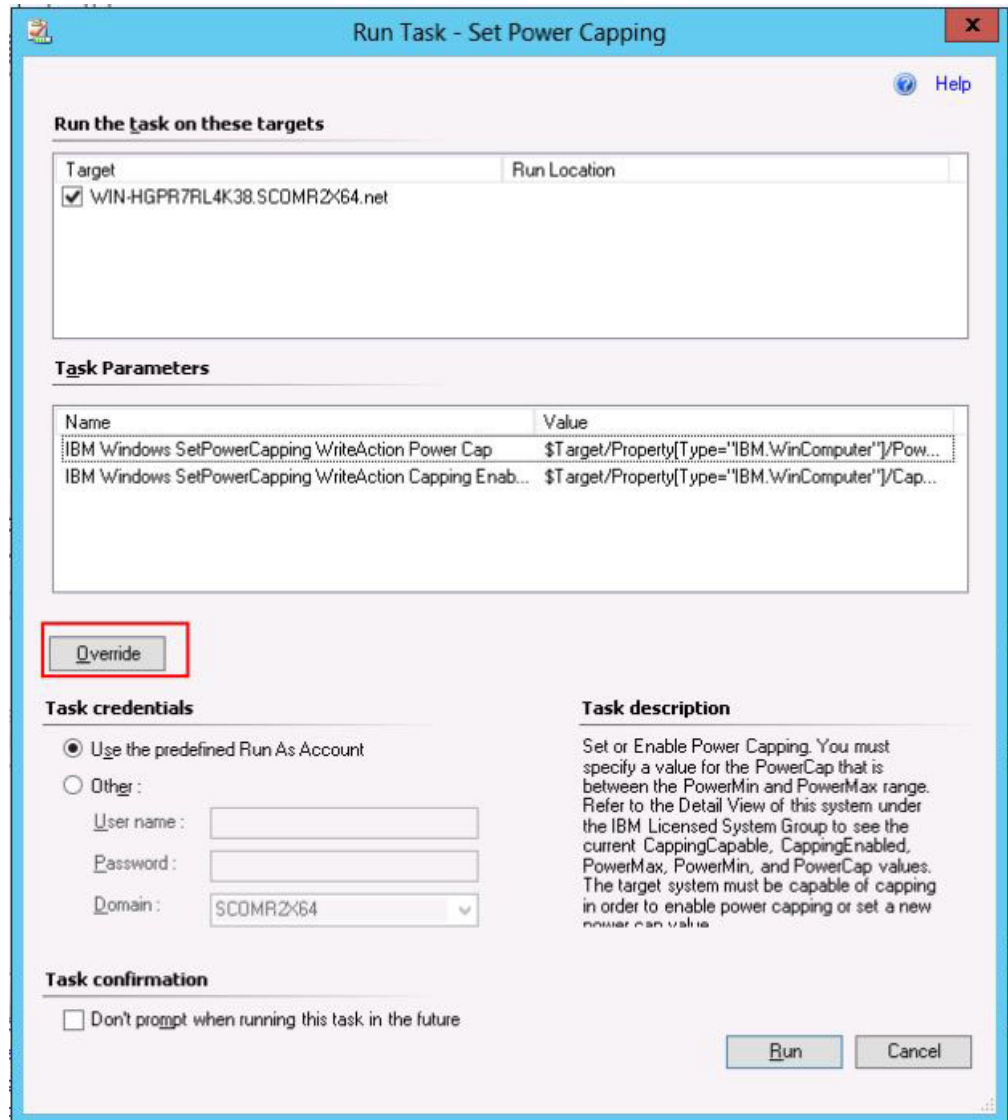


Figure 67. Target and task parameters of the Set Power Capping task

5. Click **Override** to override the power threshold values.

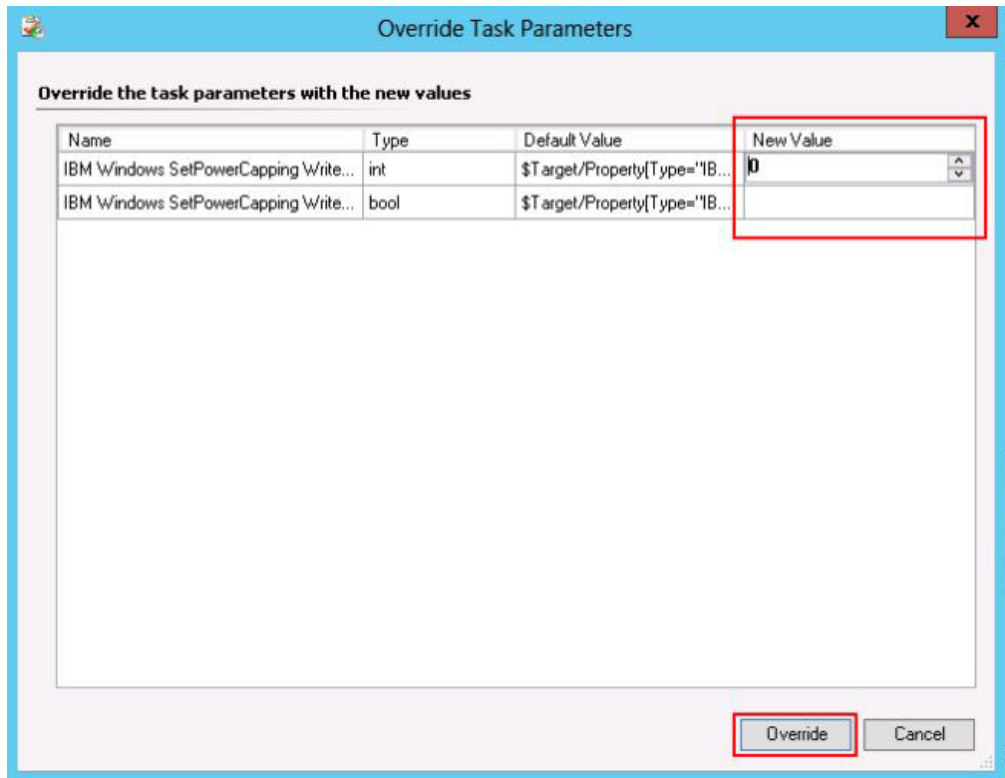


Figure 68. Override the Task Parameters of Set Power Capping task

6. Enter new values for the power capping parameters and click **Override**.
7. Verify the values that you just set in the middle pane.

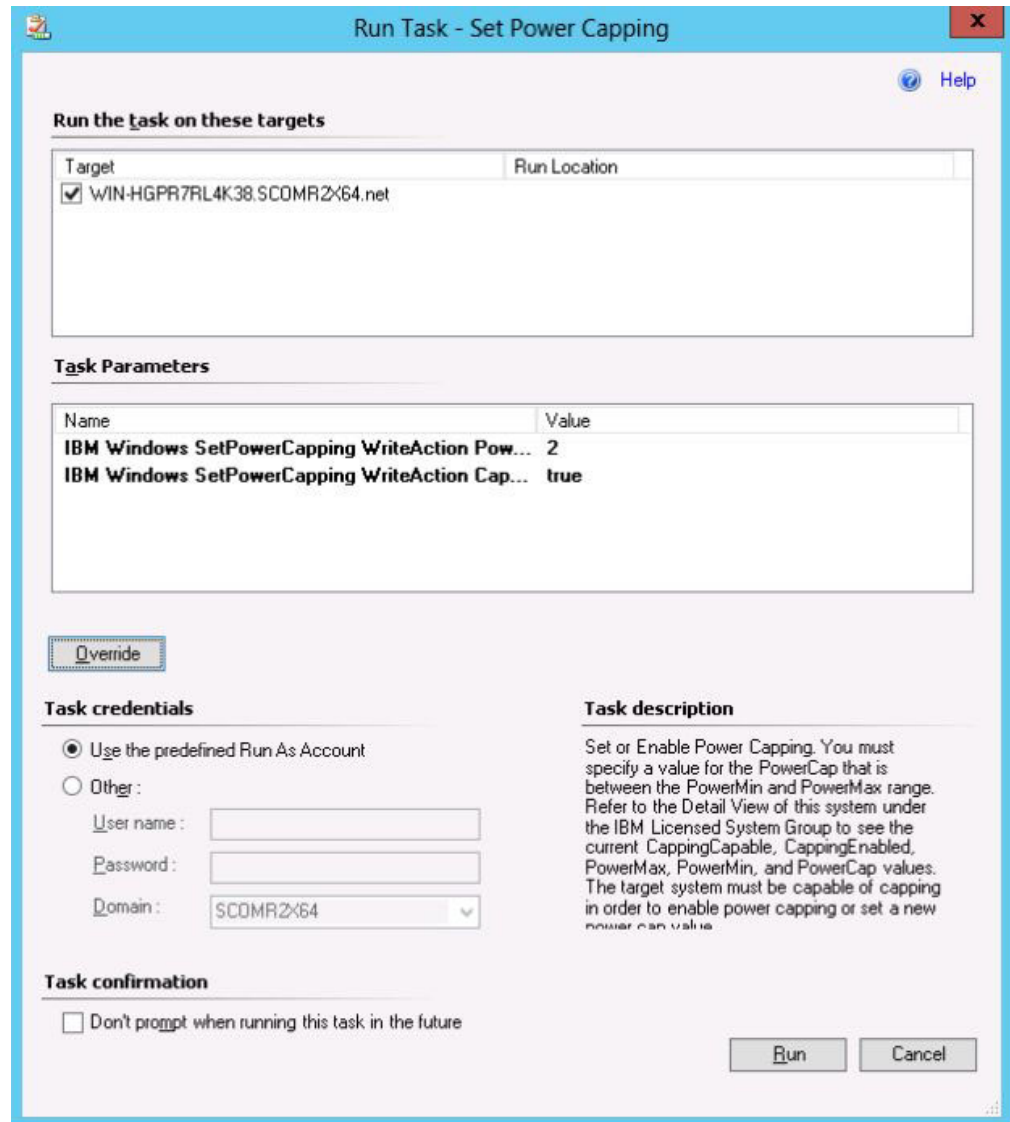


Figure 69. New values of the Task Parameters of Set Power Capping task

- After entering the new values, click **Run**. The task status window indicates the task has been sent to the target server.

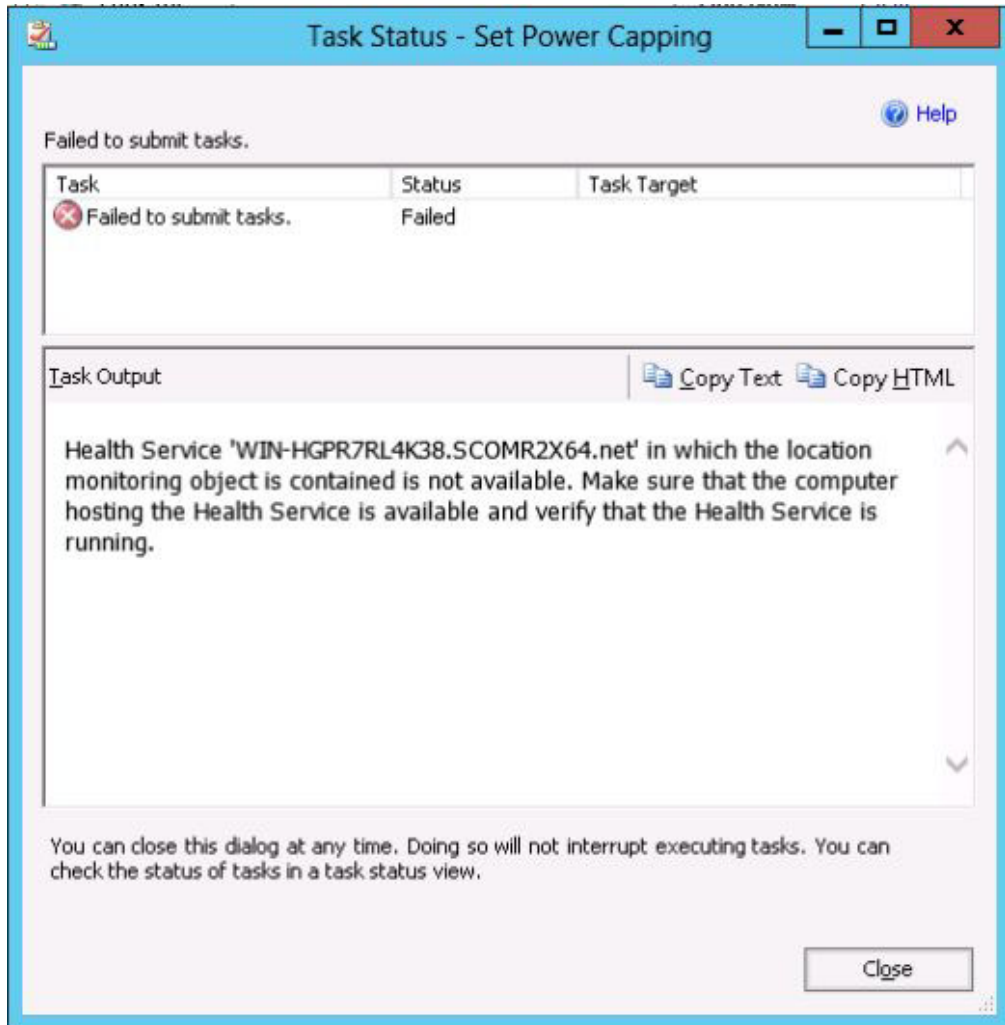


Figure 70. Task Status indicating the Set Power Capping task has been sent to the target server

A message is displayed in the Task Output section indicating whether the task succeeded or failed.

9. Click **Close**.

## Setting the Predictive Failure Alert (PFA) Policy

IBM Hardware Management Pack for Microsoft System Center Operations Manager, v5.5 provides an automatic virtual machine (VM) evacuation method if a hardware failure occurs on a host server. The following procedure provides instructions and an example of how to set the Predictive Failure Alert (PFA) Policy.

### Before you begin

To execute this task, the target system must be capable of predictive failure alerts. Currently, only Brickland-based systems support this task. To determine whether a machine supports predictive failure alert settings, check the *IMM RAS Supported* property found in the IBM Integrated Management Module (IMM) section of the Operations Manager Console. If a machine supports PFA Policy, the automatic virtual machine evacuation is based on the hardware failure alerts selected in the following procedure.

### About this task

This task is performed from the Operations Manager Console.

### Procedure

1. Click **Monitoring** > **IBM Hardware** > **IBM Integrated Management Module (IMM)**.
2. In the **IBM Integrated Management Module (IMM)** view located in the top center pane, select a server that indicates it is *IMM RAS Supported* as shown in the following figure.

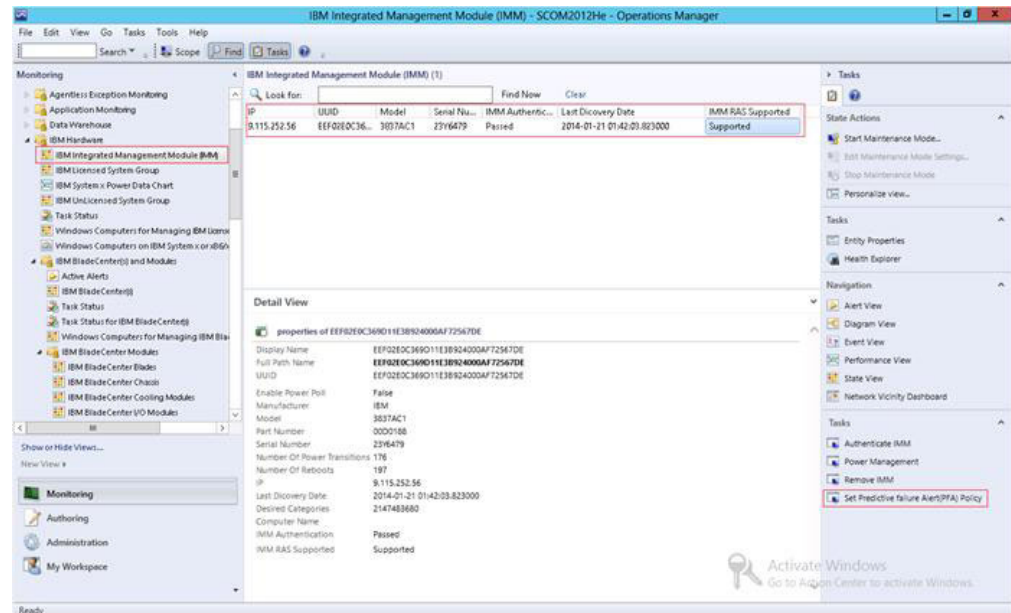


Figure 71. Set Predictive Failure Alerts Policy task example

3. In the **Actions** pane, select **Set Predictive Failure Alert (PFA) Policy** . The PFA Policy Configuration window opens.

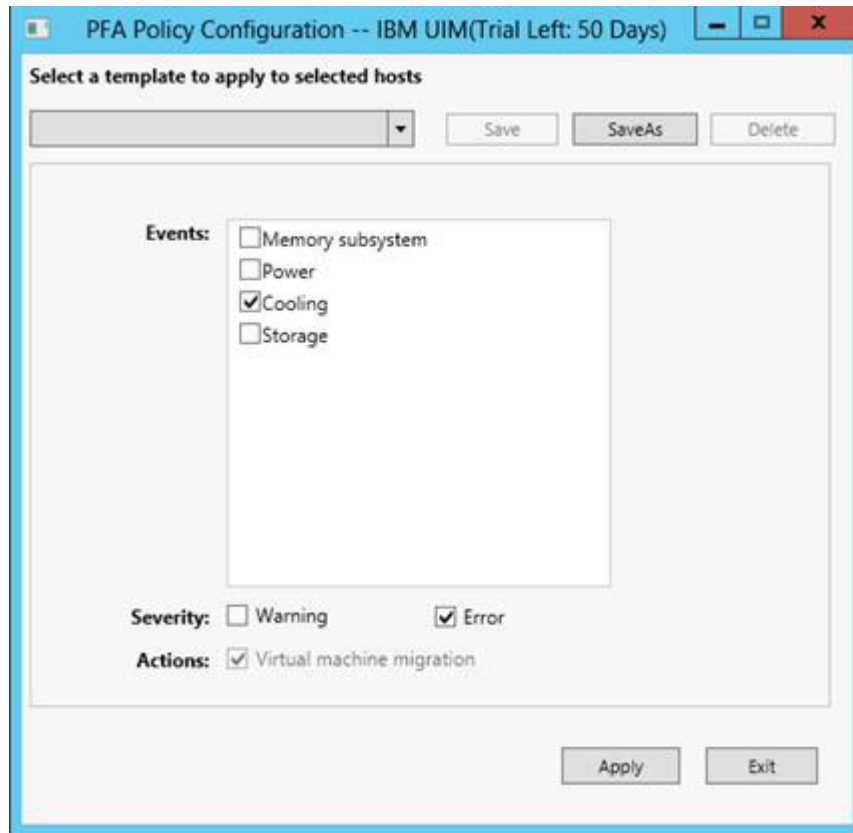


Figure 72. PFA Policy Configuration window

4. In the PFA Policy Configuration window, complete the following, applicable steps:
  - To create a new template:
    - a. From the **Select a template to apply to selected hosts** list, select a template.
    - b. From the **Events** list, select the applicable hardware failure alert events.

**Note:** The **Events** list is dependent on what types of alert events are supported by the target server. For example, IBM System x3850 X6 supports the follow alert events:

      - Memory subsystem
      - Power
      - Cooling
      - Storage
    - c. Select the severity level for the alert:
      - Warning
      - Error
    - d. If applicable, select **Virtual machine migration**.



**Note:** To automatically perform virtual machine migration, you should first set **SCVMM FQDN**. Refer to Step 7 in “Steps for installing the IBM Hardware Management Pack” on page 20.

- e. Click **Save As**.
- To modify an existing template:
  - a. From the **Select a template to apply to selected hosts** list, select an existing template.
  - b. In the **Events** list, make any necessary changes, by selecting and deselecting events.
  - c. If applicable, modify the severity level for the alert.
  - d. If applicable, select or deselect the **Virtual machine migration** option.
  - e. Click **Save**.
- Click **Delete** to remove an existing template.

## Viewing the power data for client System X servers

The IBM System x Power Data Chart feature offers you the ability to view the power data of client System x servers in an intuitive chart. The power data chart feature is only available on IBM System x servers and is not available on Chassis and Flex systems.

### Before you begin

Before you view the data chart, you should have at least one managed System x server with the Windows operating system installed on it.

### About this task

This task is performed from the Operations Manager Console.

### Procedure

1. Click **Monitoring > IBM Hardware > IBM System x Power Data Chart**.
2. Select the server check box. The IBM System x Power Data Chart is displayed.

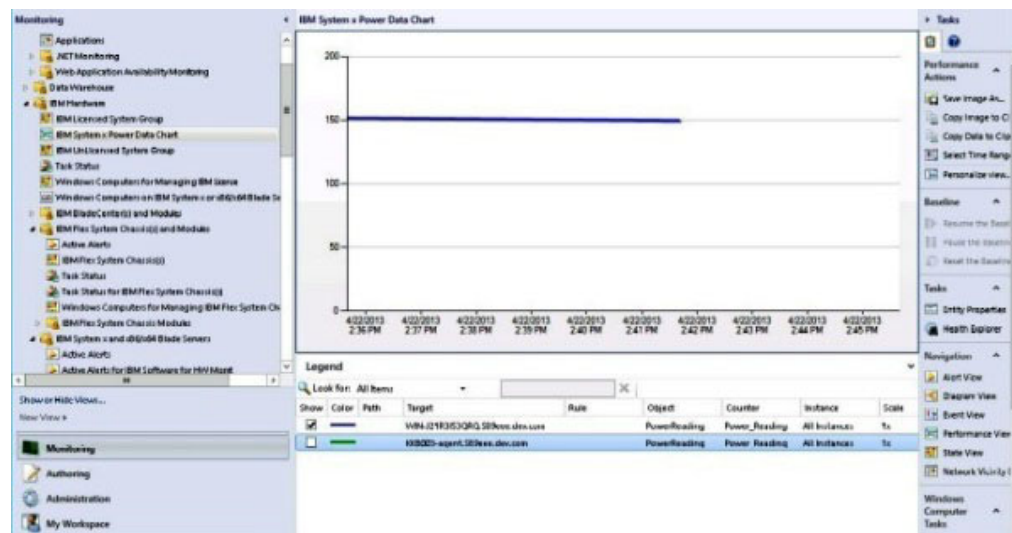


Figure 73. IBM System x Power Data Chart

Unless there are power fluctuations, the power usage is displayed as a straight line.

## Discovering the Flex System OOB-IB Reflection

If both the Flex chassis and Flex systems in a chassis have Windows operating system installed on it and are managed by the Operations Manager, the IBM Hardware Management Pack offers you the ability to synchronize information you get from the Flex chassis and system operating system.

### Before you begin

To ensure that the OOB-IB Reflection information is available, the Flex chassis device and at least one Flex system within it should be discovered and managed by the Operations Manager with the IBM Hardware Management Pack.

### About this task

This task is performed from the Operations Manager Console.

### Procedure

1. Click **Monitoring > IBM Hardware > IBM Flex System Chassis(s) and Modules** to verify that the target Flex chassis was discovered. If the target Flex Chassis was not discovered, refer to “Discovering an IBM Flex System in Operations Manager 2012” on page 51.

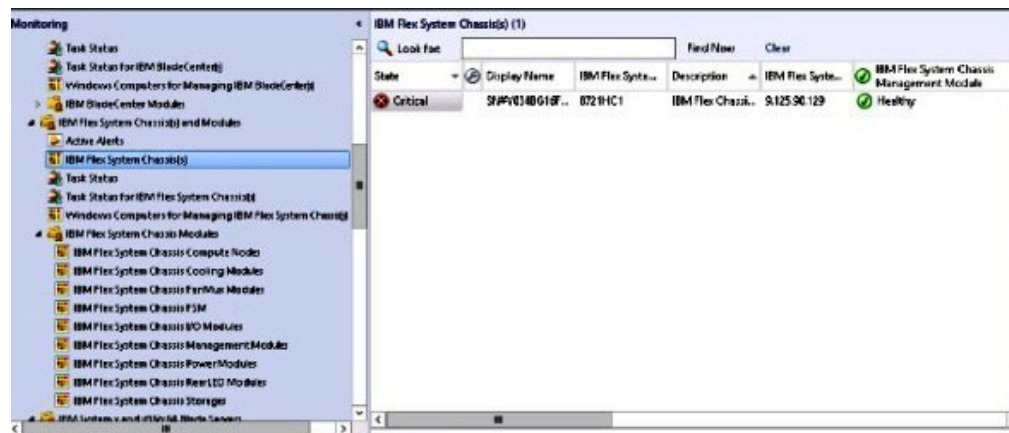


Figure 74. Check IBM Flex System Chassis

2. Click **Monitoring > IBM Hardware > IBM Flex System Chassis Modules > IBM Flex System Chassis Compute Nodes** to verify that the nodes in the Flex system were successfully discovered by the Operations Manager.

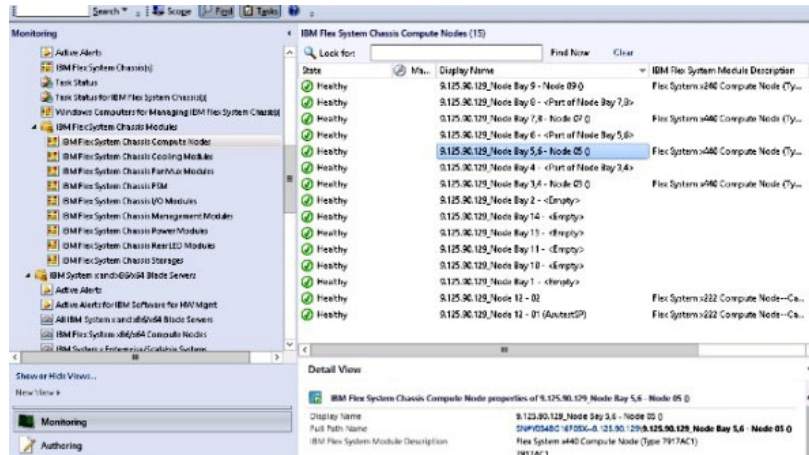


Figure 75. Checking IBM Flex System Chassis Compute Nodes

3. Click **Monitoring > IBM Hardware > IBM Licenses System Group** to verify that the target Flex system was discovered by the Operations Manager. If the target Flex system was not discovered by the Operations Manager, refer to “Adding an IBM system that will be managed by the Operations Manager” on page 61.

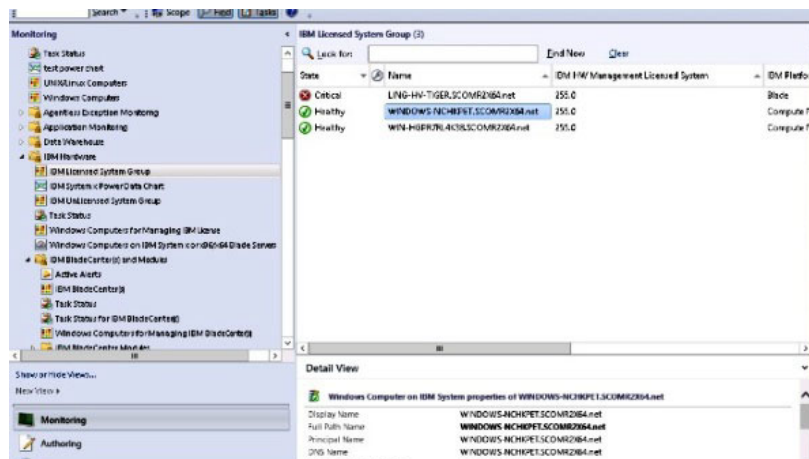


Figure 76. Example of an IBM Licensed System Group

- Click **Monitoring > IBM Hardware > IBM System x and x86/64 Blade Servers > IBM x86/64 Flex OOB-IB Reflection Group**. The OOB-IB Reflection information is displayed.

**Note:** It may take some time to establish the OOB-IB Reflection after the Flex chassis and Flex system was discovered.

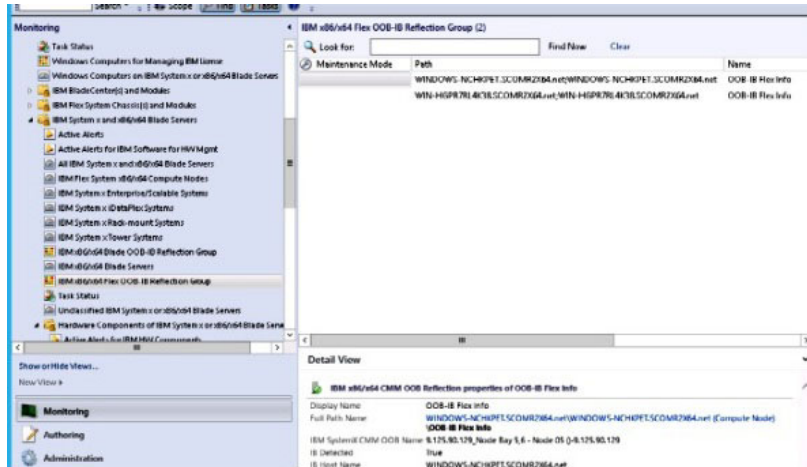


Figure 77. Example of an IBM x86/64 Flex OOB-IB Reflection Group

## Using Flex system remote power on and off

The Flex system remote power on and off premium feature allows you to remotely control the IBM Flex system to power on, power off, or shut down the operating system. When this feature is enabled, the options are listed in the Actions pane of the Operations Manager Console.

### About this task

This task is performed from the Operations Manager Console.

### Procedure

- Click **Monitoring > IBM Hardware > IBM Flex System Chassis(s) and Modules > IBM Flex System Chassis Modules > IBM Flex System Chassis Compute Nodes**.
- In the Actions pane, select one of the following options for the selected Flex system:

**IBM.FlexSystem.PowerOn.Blade:**

To power on

**IBM.FlexSystem.PowerOff.Blade:**

To power off

**IBM.FlexSystem.SoftPowerOff.Blade:**

to soft power off

The following figure provides an example of IBM Flex System Chassis Compute Nodes.

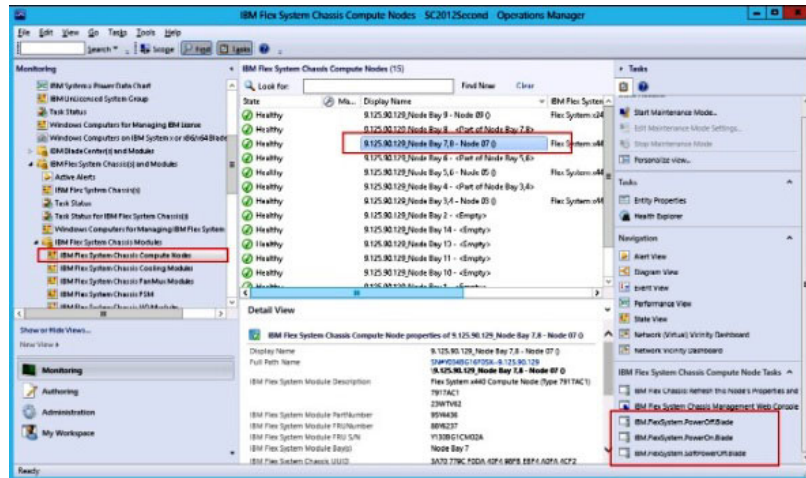


Figure 78. Example of remote power options for IBM Flex System Chassis Compute Nodes

3. Optional: To use the power on option, from the **IBM Flex System Chassis Compute Node Task** list located in the lower right pane, select **IBM.FlexSystem.PowerOn.Blade**. The Run Task - IBM.FlexSystem.PowerOn.Blade window is displayed. By default, the target server and account are selected.

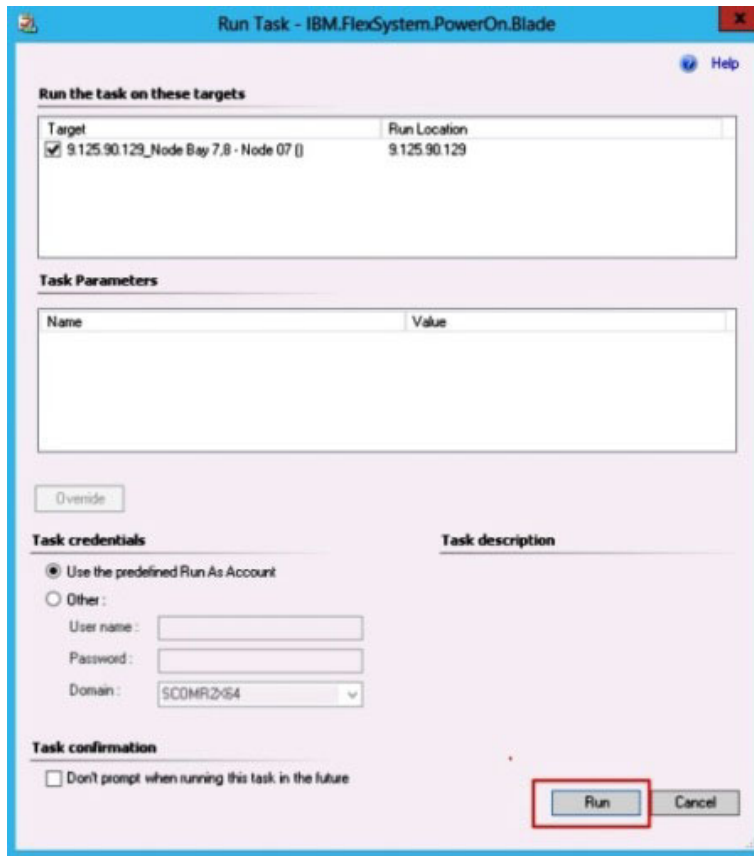


Figure 79. Window for remote power on task for Flex systems

4. Click **Run** to launch the task.  
After the power-on task has finished, the task status is displayed.

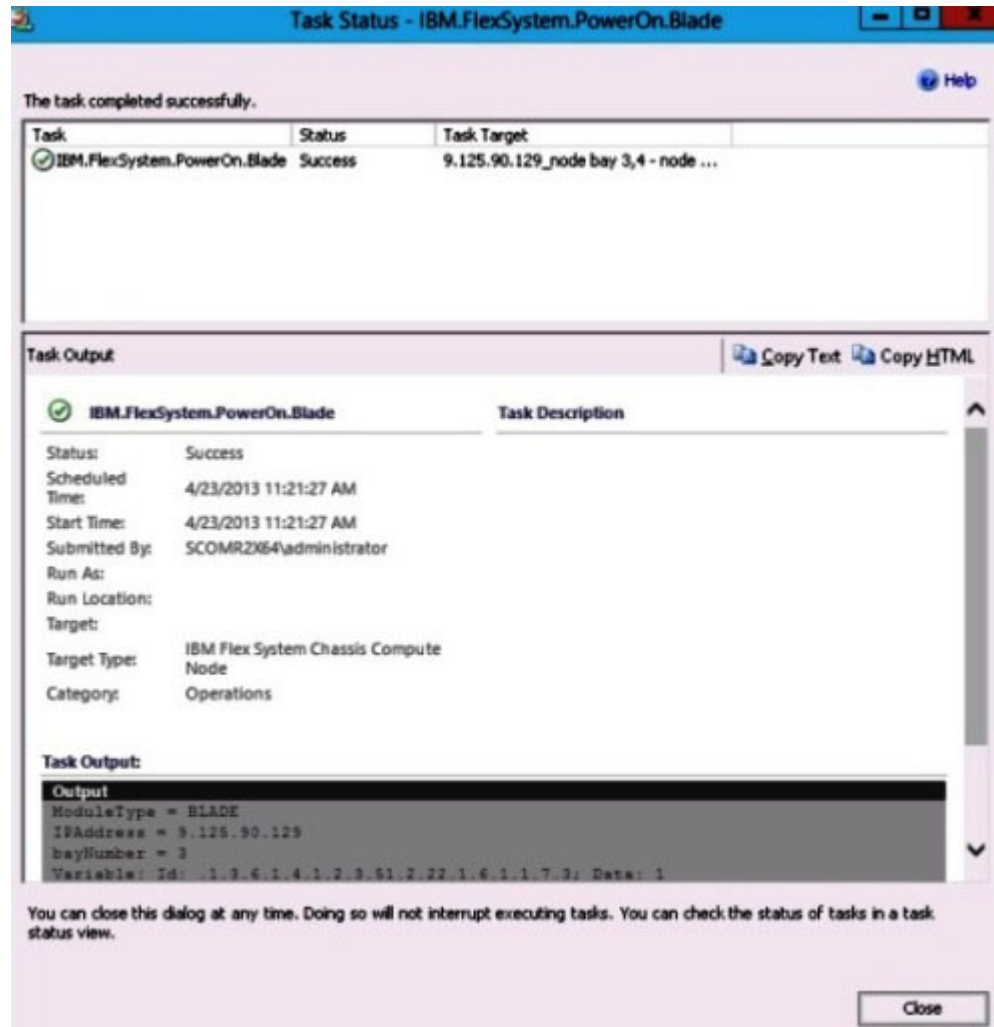


Figure 80. Task status for remote power on

**Note:** When the premium feature is not enabled, the task fails. A message is displayed in the Task Output section indicating that the free version of the IBM Hardware Management Pack is being used, as shown in the following figure.

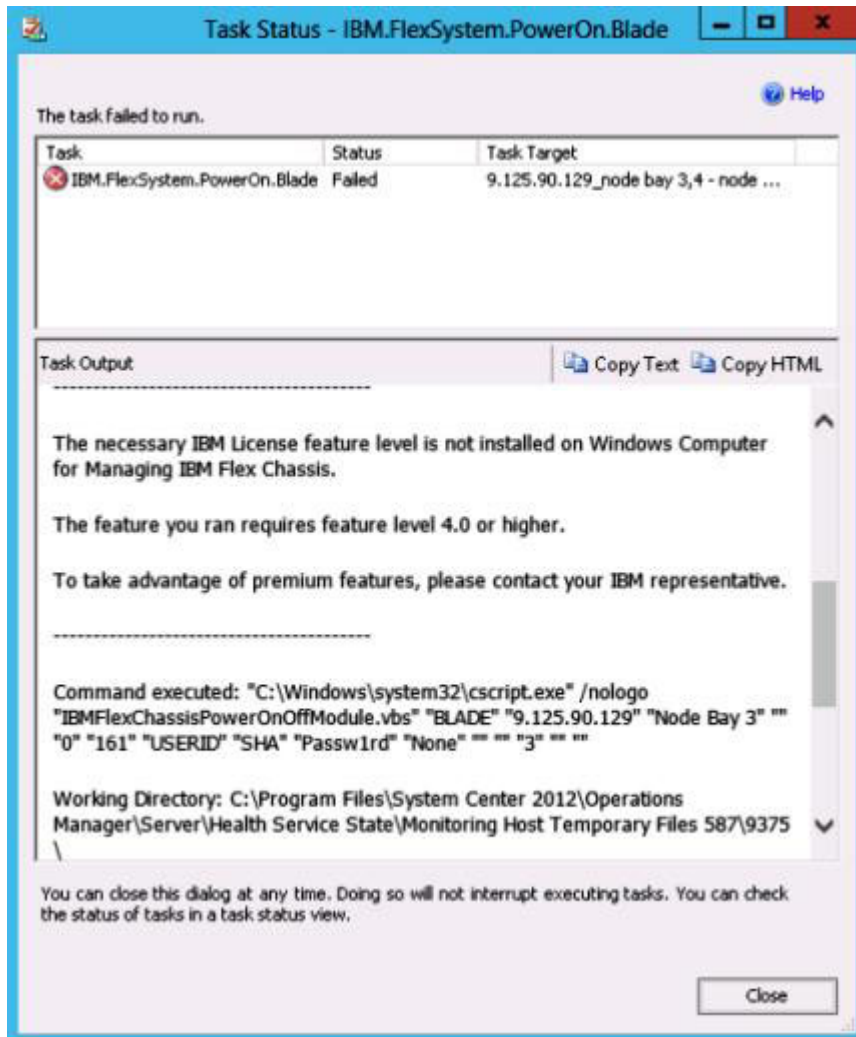


Figure 81. Task Status indicating power on failed because no license is installed

5. Click **Close** to exit the task status window.

## Launching the IBM Flex System Chassis Web Console

When the premium feature for launching the Flex System Web Console is enabled, this task is available in the Action pane of the Operations Manager Console. This feature allows you to launch the Flex System Chassis Web Console by using links inside of the Operations Manager Console.



## About this task

This task is performed from the Operations Manager Console.

## Procedure

1. Click **Monitoring > IBM Hardware > IBM Flex System Chassis(s) and Modules > IBM Flex System Chassis(s)**.
2. Click the target Flex System Chassis.
3. From the Actions pane located on the right, click **IBM Flex System Chassis Management Web Console**.

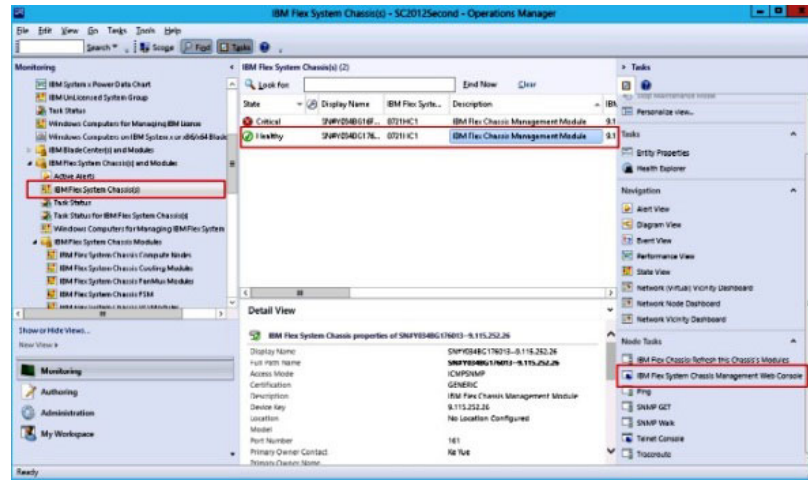


Figure 82. Example of launching the IBM Flex System Chassis Management Web Console

4. Click **Continue to this website** and trust this website.

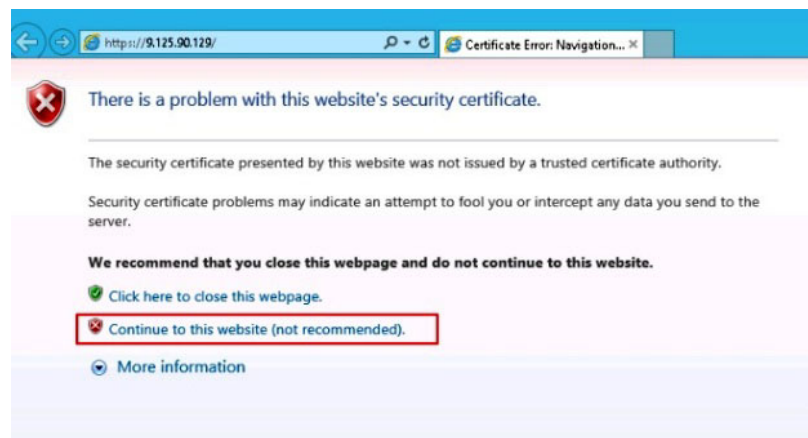


Figure 83. Certificate error when opening IBM Flex System Chassis Management Web Console

If the Flex System Chassis web page is not trusted by your browser, and if the CMM configuration is correct, this page will disappear and the CMM Web Console will open in your default browser.

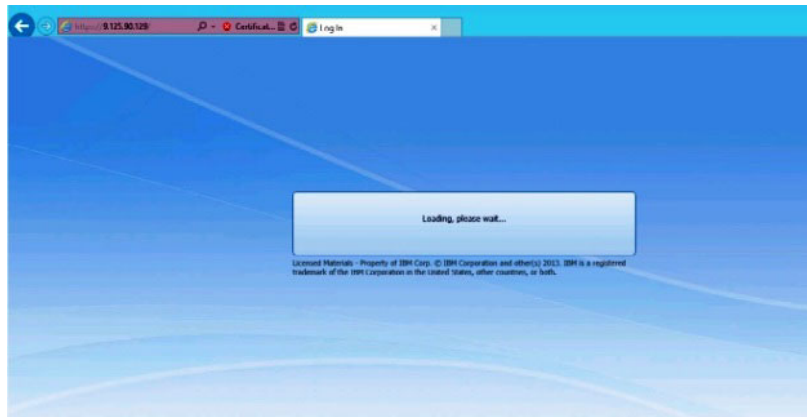


Figure 84. Loading CMM Web Console

When the CMM Web Console has successfully loaded, the following window is displayed.



Figure 85. CMM Web Console

5. To log in to the CMM Console, complete the following steps
  - Enter the User name and Password.
  - From the **Interactive session timeout interval** list select a value or use the default value of *no timeout*.
  - From the **Select an automatic refresh** list, select a refresh value or use the default value of *no refresh*.
  - Click **Log In**.

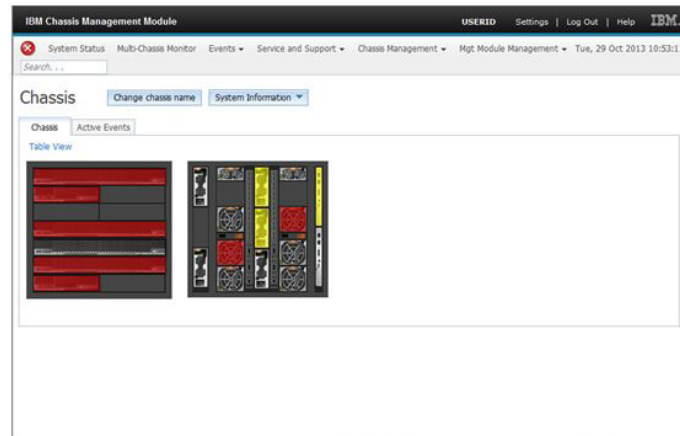


Figure 86. CMM Console

## Discovering an IBM Flex System Chassis FSM

When the premium feature for discovering an IBM Flex System Manager (FSM) system is enabled, the **Discovering an IBM Flex System Chassis FSM** task is available in the Actions pane of the Operations Manager Console. This feature allows you to discover and manage an FSM system in the Operations Manager Console.

### About this task

This task is performed from the Operations Manager Console.

### Procedure

1. Click **Monitoring > IBM Flex System Chassis Modules > IBM Flex System Chassis FSM**. In the results pane, a list of all the IBM Flex System Chassis FSMs is displayed.

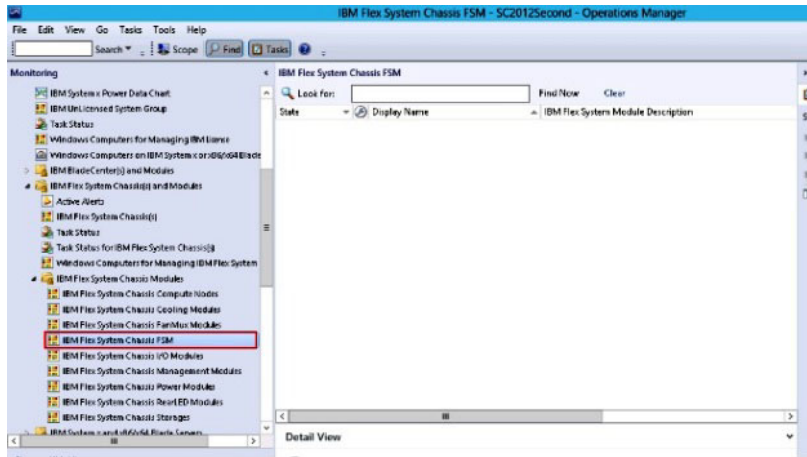


Figure 87. Example of an IBM Flex System Chassis FSM

2. Verify the target FSM is included in the list. If the target FSM is not included in the list, verify that the Flex system chassis containing the FSM has been discovered by completing the following steps.
  - a. Click **Monitoring > IBM Flex System Chassis(s) and Modules > IBM Flex System Chassis(s) > IBM Flex System Chassis**. The results pane displays the IBM Flex System Chassis and their status.
  - b. In the Actions pane, select an **IBM Flex System Chassis** and run the Node task: **IBM Flex Chassis: Refresh this Chassis's Modules**. The target FSM system is discovered and displayed in IBM Flex System Chassis FSM list.

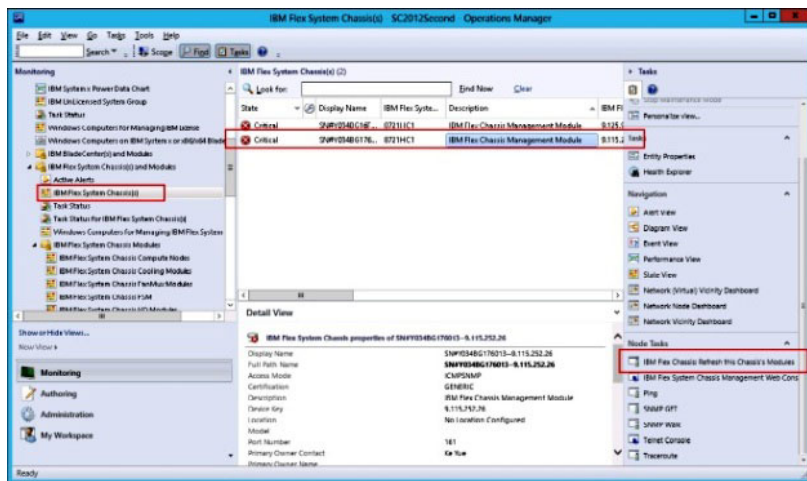


Figure 88. Refreshing the Chassis's Module

## Launching the IBM Flex System Chassis FSM Web Console

When the premium feature for launching the IBM Flex System Chassis FSM Web Console is enabled, this task is available in the Actions pane of the Operations Manager Console. This feature allows you to launch the Flex chassis Flex System Manager (FSM) Web Console by using links inside the Operations Manager Console.

### About this task

This task is performed from the Operations Manager Console.

### Procedure

1. Click **Monitoring** > **IBM Flex System Chassis Modules** > **IBM Flex System Chassis FSM**.
2. In the results pane, select the target **IBM Flex System Chassis FSM**, and then in the **Tasks** list in the Actions pane, select the **Set FSM IP Address**.

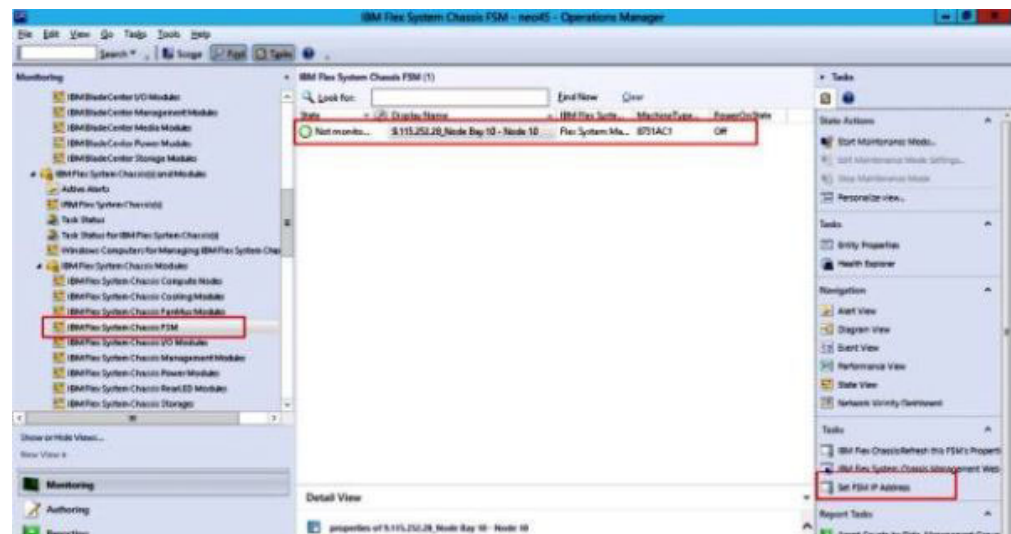


Figure 89. Example of setting the FSM IP address from the SCOM console

3. In the Run Task - Set FSM IP Address window, click **Override**.



Figure 90. Run Task - Set FSM IP Address window

The Override Task Parameters page is displayed.

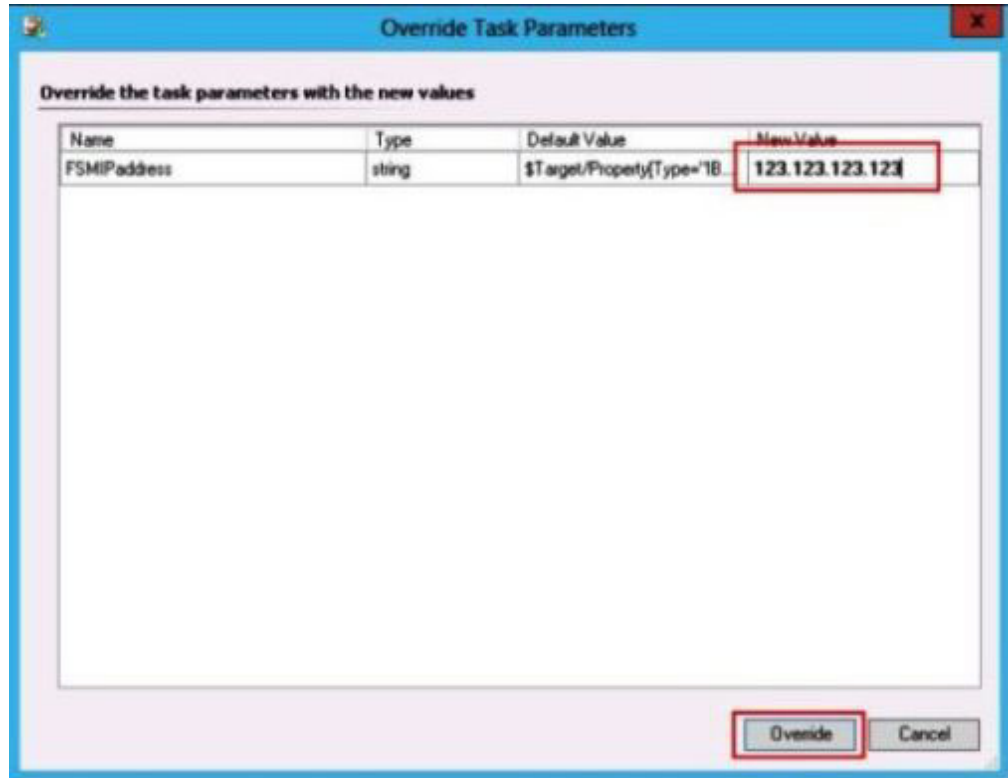


Figure 91. Example of overriding FSM IP address

4. In the **New Value** field, enter the correct IP address of the target FSM and click **Override**. You can get the FSM IP address from the Flex System Chassis Web Console.
5. In the Task - Set FSM IP Address window, click **Run**. The Set FSM IP Address window is displayed indicating the task status.

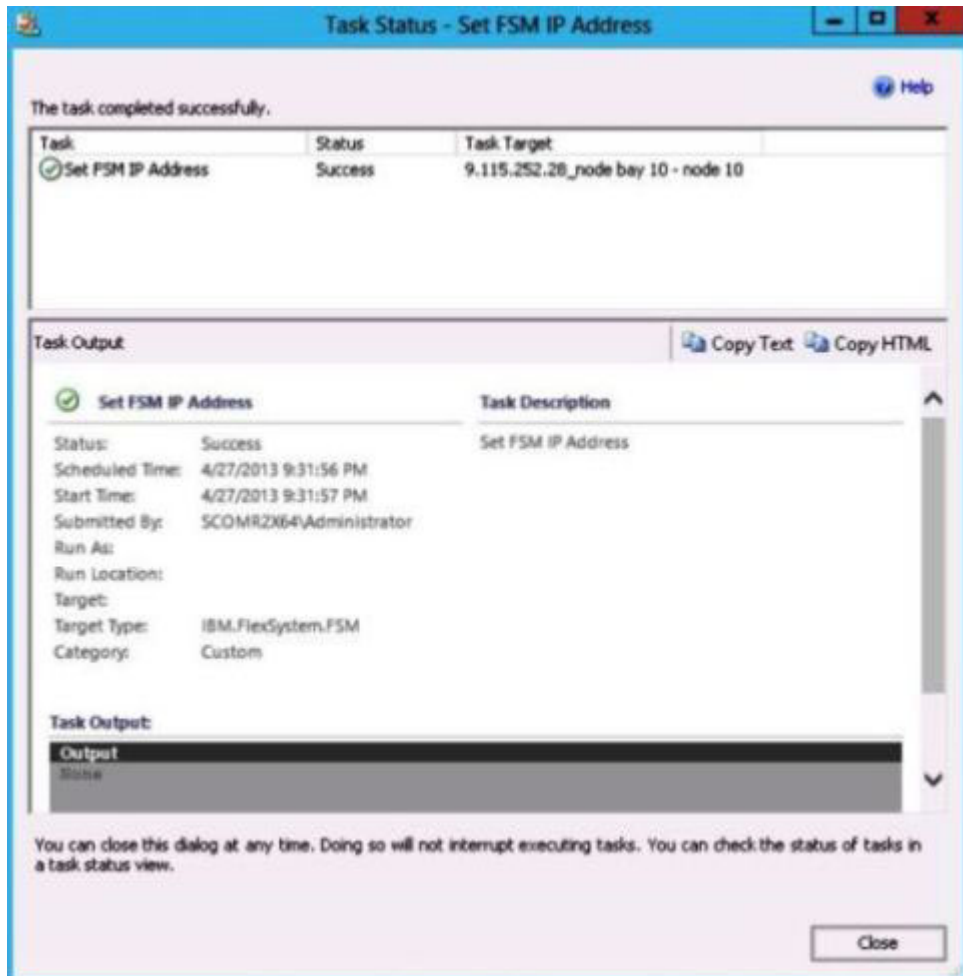


Figure 92. Task Status of Setting FSM IP Address indicating the task successfully completed

6. Click Close.

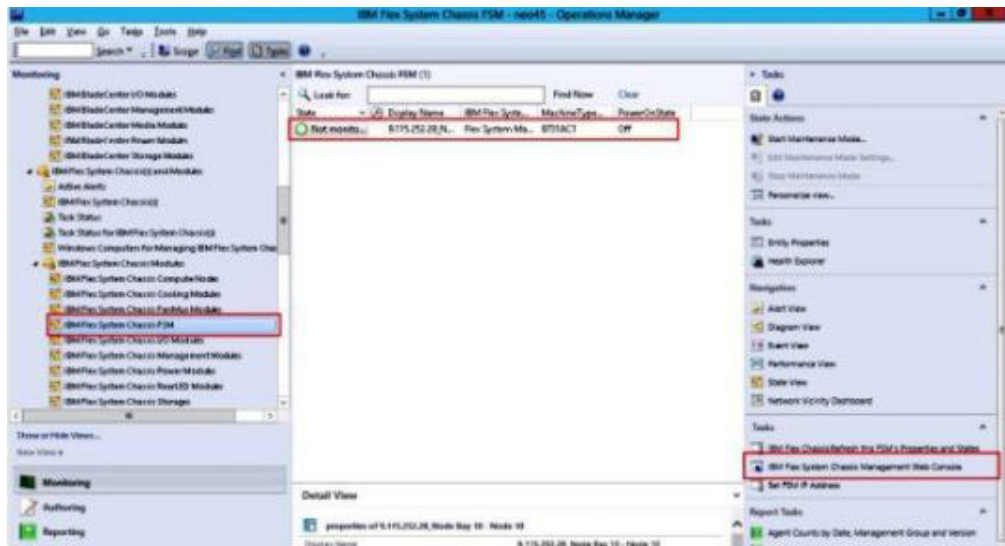


Figure 93. Example of launching an FSM Web Console from the SCOM console



7. In the Actions pane, select **IBM Flex System Chassis Management Web Console**.

The Operations Manager opens the FSM Web Console in your default browser.



Figure 94. FSM Web Console log in



---

## Chapter 6. Working with Hardware Failure Management

The topics in this section describe how the IBM Hardware Management Pack enhances the RAS ability to manage IBM IMMv2 or later versions of the hardware products by using Hardware Failure Management.

The Hardware Management Pack provides the following functionality for Hardware Failure Management:

- Discovery of an Integrated Management Module (IMM) and the ability to correlate it with the host.
- IMM authentication and the ability to obtain information through the IMM CIM.
- IMM deletion option.
- Power management implementation.
- Setting a Predictive Failure Alert Policy for an IMM.

**Note:** This function will only work in SCOM 2012 and later versions. It cannot be used with SCOM 2007 R2.

---

### Enabling Hardware Failure Management using the Operations Manager Console

The following procedures describe how to enable the Hardware Failure Management feature using the Operations Manager Console with the IBM Hardware Management Pack installed.

#### About this task

By completing the following tasks, you can enable the Hardware Failure Management feature:

- IMM discovery and authentication and inventory - SLP
- IMM authentication and inventory - CIM

---

### IMM discovery and authentication

The Hardware Management Pack leverages the System Center Operations Manager's task for discovering an IMM2 node.

## About this task

This task is performed from the Operations Manager Console.

## Procedure

1. Click **Windows Computers**. In the middle pane, the IBM Integrated Management Module Discover Console is displayed.

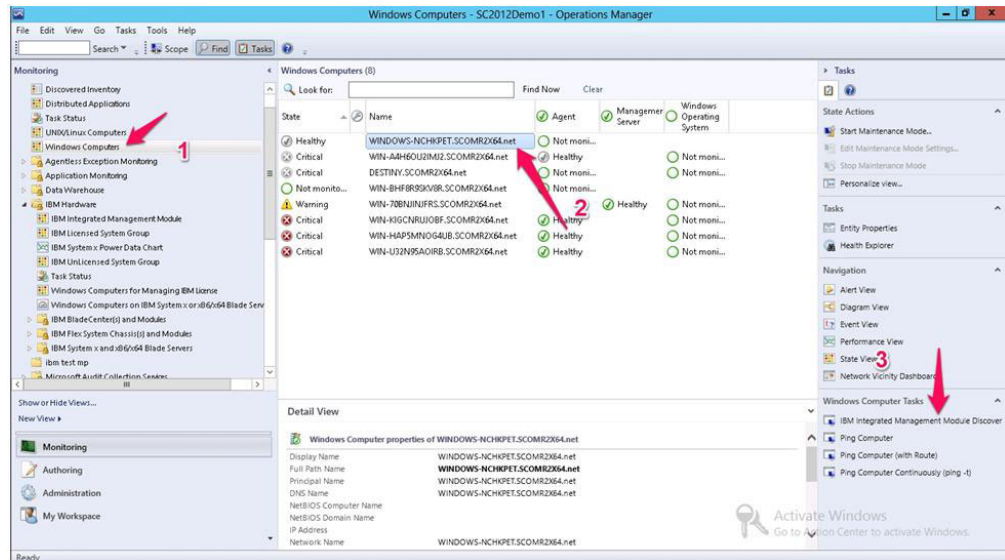


Figure 95. IMM Discover Console

2. In the Windows Computer Tasks section located in the bottom right side of the screen, click **IBM Integrated Management Module Discover**. The IMM Discovery page opens.

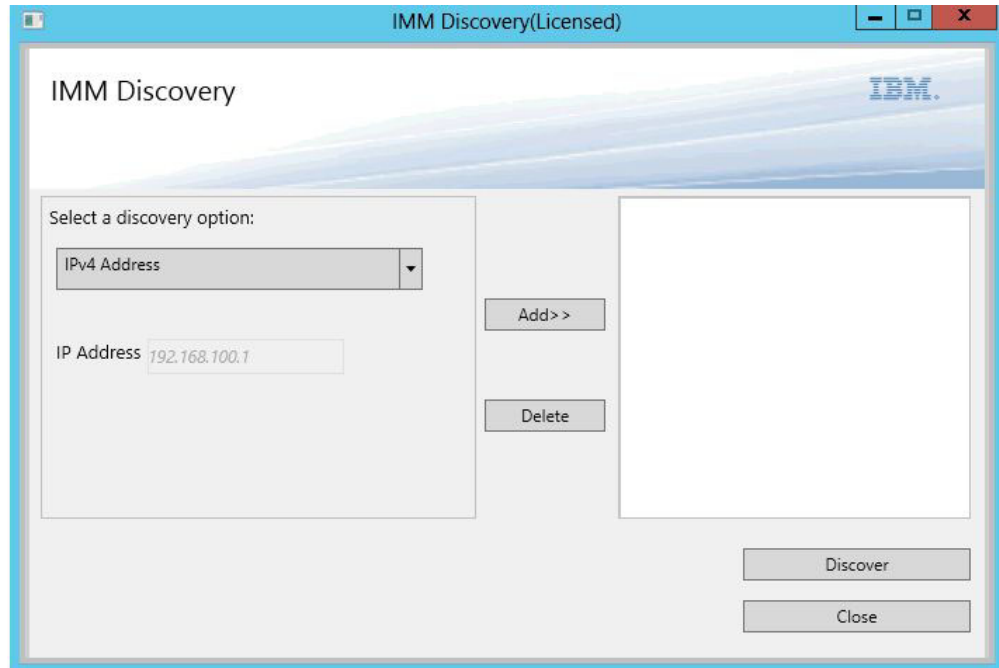


Figure 96. IMM Discovery

3. Using the dual-list, perform the following steps to create an IMM discovery list:
  - a. On the left side, select one of the following two discovery options from the list: **IPv4Address** or **IPv4Range**.
  - b. In the IP Address field, enter the IPv4Address or the IPv4Range.
  - c. Click **Add**.
  - d. Click **Discover**.

This task may take several minutes to discover all of the Integrated Management Modules and for Operations Manager to perform a query of discovered data.

When the IMM discovery is finished, the IMM nodes are displayed in the IBM Integrated Management Module pane.

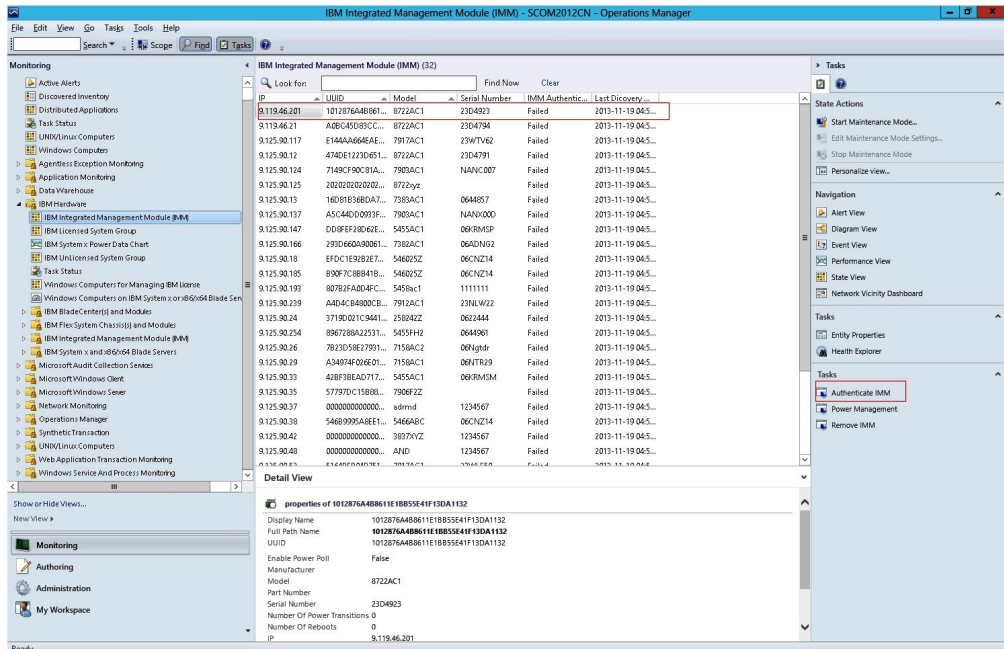


Figure 97. Integrated Management Module

4. Click an IMM node. A corresponding task list is displayed on the right
5. From the Tasks list, select **Authenticate IMM**.  
The IMM Authentication dialog box opens.



Figure 98. IMM Authentication

6. Enter the User name and Password, then click **Connect**.

**Note:** Due to an IMM security policy limitation, IMM Authentication will only try to authenticate the User name and Password twice. After two incorrect attempts, the IMM log in username is locked.

---

## Using the power management feature for Hardware Failure Management

A discovered Integrated Management Module (IMM) supports the basic power management feature. The power management feature only supports a rack-type server. Power capping of BladeCenter and Flex systems are integrated by using the Advanced Management Module (AMM) and the Chassis Management Module (CMM).

### Procedure

1. Select the IMM instance and then from the **Tasks** list, select **Power Management**. The Power Capping Management dialog box is displayed.

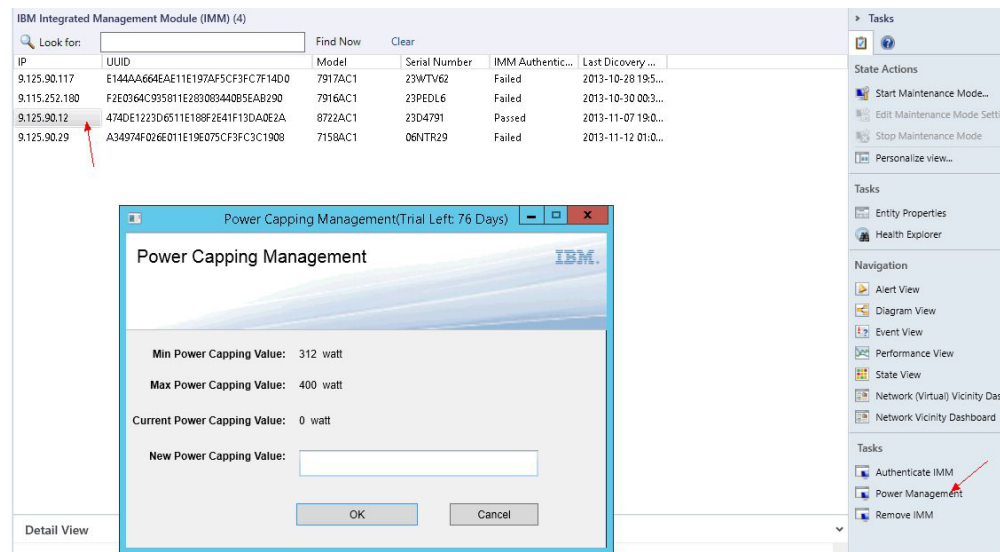


Figure 99. Power Capping Management

2. Enter a **New Power Capping Value** and then click **OK** to save that value or **Cancel** to not save a new power capping value.





## Appendix A. Best practices

The topics in this section provide suggested methods for completing tasks.

### Best practice: Determining the cause of an error

Use the following diagnostic procedure to identify and solve problems that might occur in a managed environment.

#### About this task

This task is performed from the Operations Manager Console.

#### Procedure

1. Click **Monitoring** to open the Monitoring navigation pane.
2. To quickly view the status of all of your managed IBM systems that have Windows operating systems, click **IBM Hardware > Windows Computers on IBM System x or x86/x64 Blade Servers**.
3. Check the health of the systems displayed in the top results pane. All newly discovered objects are in a healthy state by default. The Health check monitoring task updates the status of an object at regular intervals, according to the default interval setting. You can configure the monitoring frequency by overriding the **override-controlled** parameters. See the Microsoft System Center Operations Manager documentation about **override-controlled** for more information.
4. Select a system that shows a *Critical* or *Warning* state.

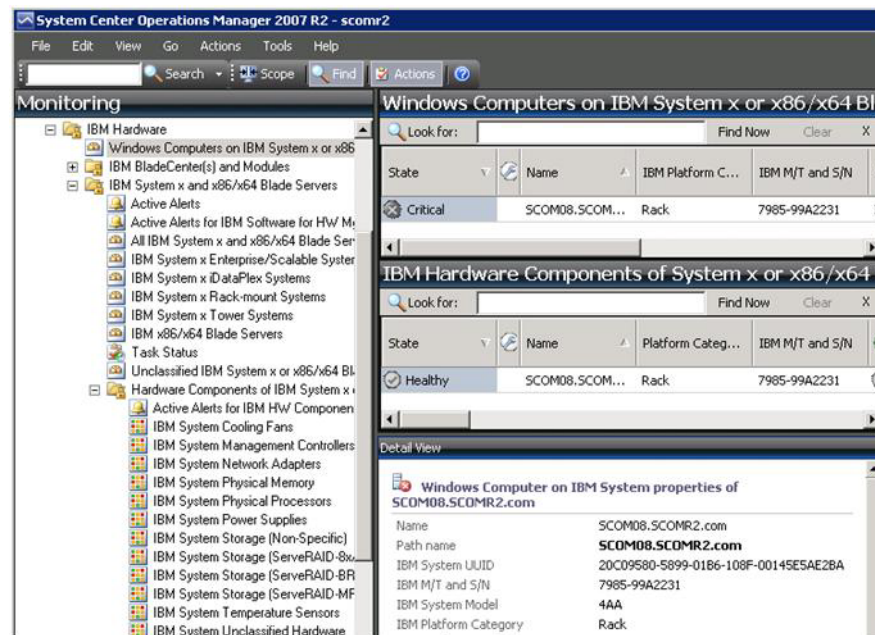


Figure 100. Example of selecting a system with a critical state

5. Determine whether the error is related to the hardware or software.
  - **Hardware-related failures:** Check the IBM Hardware Components of IBM System x or x86/x64 Blade Servers pane to select the system. Scroll to the right to view all of the component status and data. You can personalize this view.
 

This pane contains state views based on the class of the hardware component basis. The purpose of this view is to provide access to detailed properties of each component instance. Look for additional system information in the Detail View pane.
  - **Software-related failures:** Check the Windows Computer on IBM System x or x86/x64 Blade Servers pane. This pane contains state views and information on a per-software-component-class basis. Select a system that has a *Critical* or *Warning* health state.
 

The purpose of these views is to provide access to detailed properties of each component instance. The Detail View shows all instances of the system software with a health state for each of the four health aspects.
6. To obtain more information and details about a failure, access the hardware information of the desired BladeCenter module or hardware system component by clicking **IBM BladeCenter Modules**.
7. From a previous view, if you already know that a power supply component failed, select the related view, **IBM BladeCenter Power Modules**, to determine the problem with the power supply.
8. Click a **Critical** power module and review its related data.
9. Review the information and data presented in the Detailed View pane. Check all instances of the module type and each of its four health aspects.

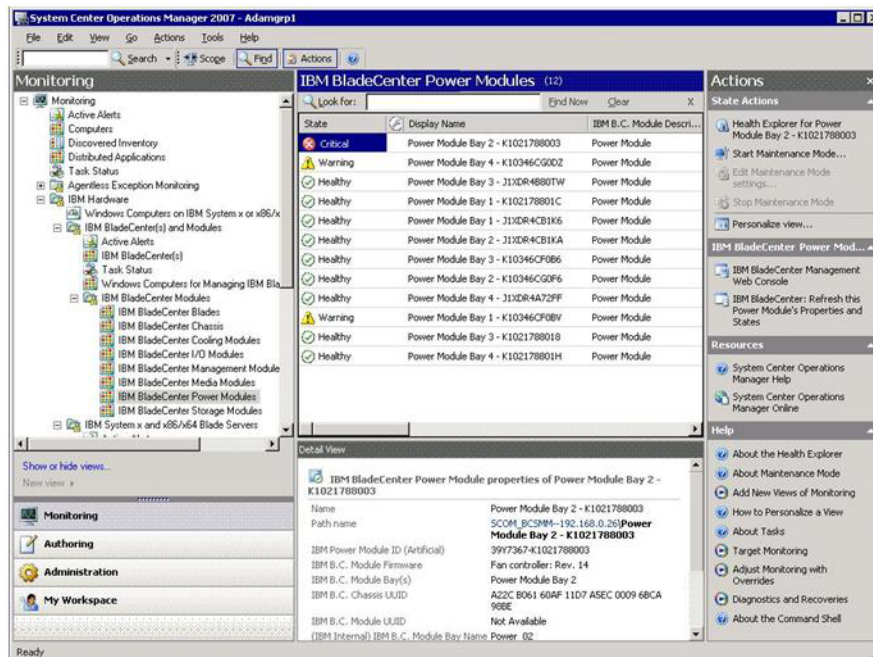


Figure 101. Detailed view of a power module in critical state

10. Right-click the **selected module** and click **open > Health Explorer**.
11. Select the alert and look at the information on the State Change Events page.
12. Depending on the type of alert you have, you can click **View Alert** for more information.
13. Click the **Knowledge** tab to read the Knowledge Page and one or more Knowledge Articles that relate to your alert.

**Important:** In addition to the health information available for each object, related information might be available from other objects that are health-related from different perspectives. For example, a blade that is monitored in-band through its platform agent shows a health state, but the BladeCenter chassis management module also shows a health state for the blade.

Other BladeCenter chassis modules might affect the blade health, such as a power supply that provides power to the blade server. Similarly, the health of a blade from the management module perspective might include the health and other information about the operating system running on the blade.

For instance, the following BladeCenter simple network management protocol (SNMP) alert has an event description field of *1.3.6.1.4.1.2.6.158.3.1.1.8* and an event ID of *1.3.6.1.4.1.2.6.158.3.1.1.14*. Convert the decimal event ID value to a hexadecimal number to look up the message in the *Advanced Management Module Message Guide*.

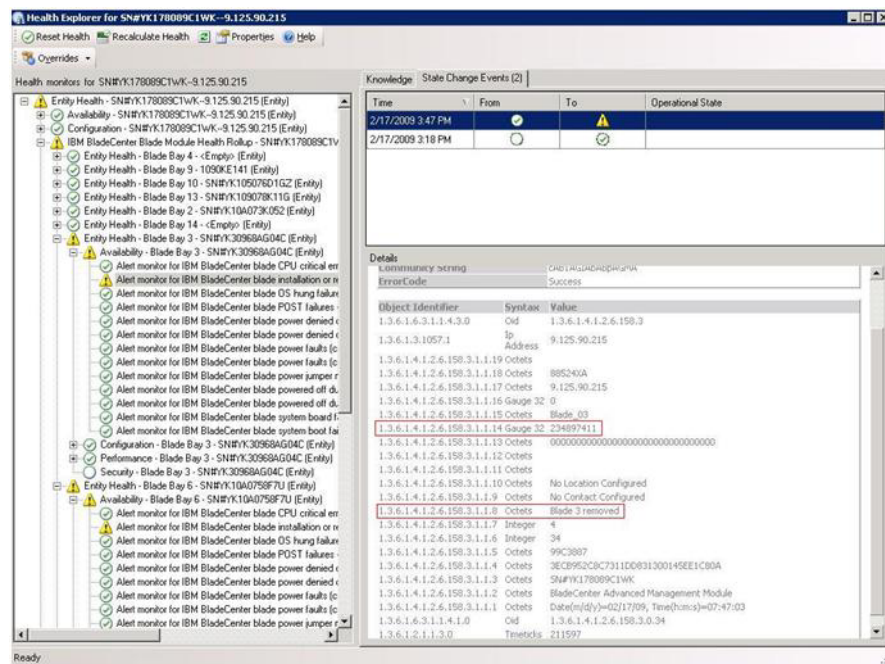


Figure 102. System x Windows Management Instrumentation (WMI) event

For a System x WMI event, the Details pane includes the event ID and a description.

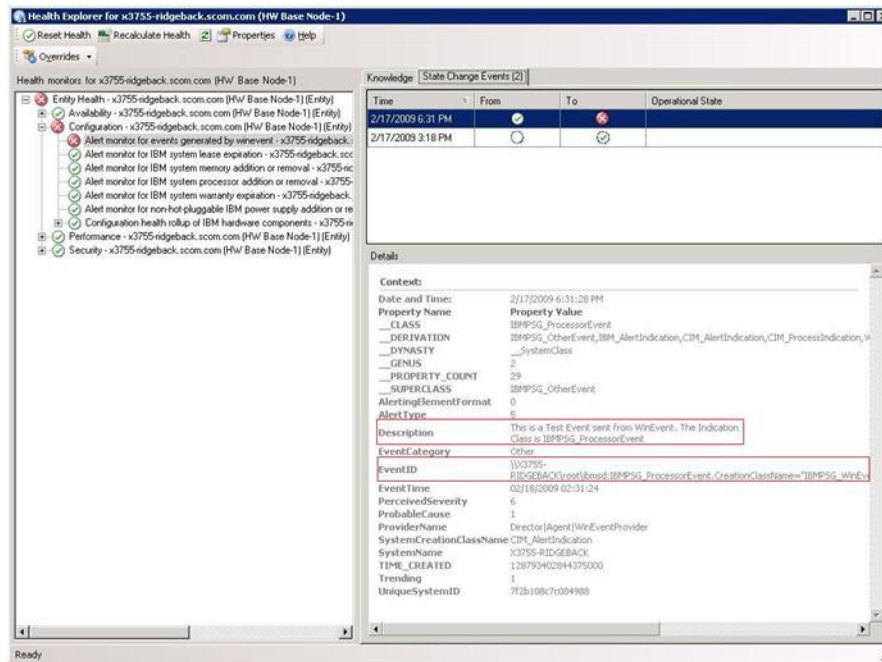


Figure 103. Example of the State Change Events tab detail information

## Best practice: Rediscovering all BladeCenters

The BladeCenter monitor stalls when the same version of the IBM Hardware Management Pack is deleted and re-imported.

### About this task

This task is performed from the Operations Manager Console.

### Procedure

1. Click **Administration > Device Management > Network Devices**.
2. Note the IP addresses listed in the Network Devices view of the results pane. You will need this information for the discovery network device information later.
3. Select the **IP Address** of the BladeCenter you want to rediscover, and in the Actions pane, select **Delete**.
4. Using the noted IP address to limit the scope of Network Devices, follow the instructions in "Discovering a BladeCenter in Operations Manager 2007" on page 34 to rediscover the BladeCenter.

## Best practice: Rediscovering a renamed server

When a Windows server is renamed, the Windows server instance entry monitored by the Operations Manager becomes grayed out. This is an indication that the Windows server is no longer being monitored by the Operations Manager.

### About this task

This task is performed in the Operation Manager's Console.

To rediscover and monitor a renamed server, first delete the original server name from the Operations Manager's Agent Managed server list, and then rediscover the renamed server by using the following procedure.

### Procedure

1. Select **Administration > Device Management > Agent Managed**.

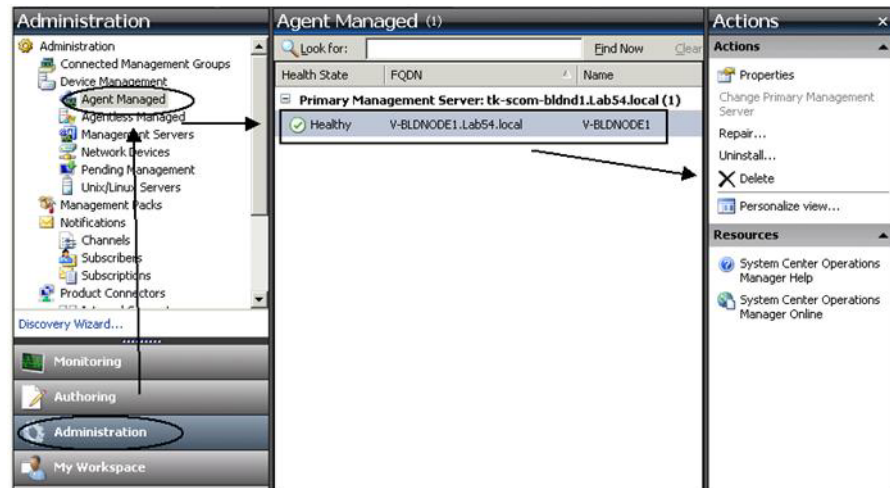


Figure 104. Deleting a renamed server

2. Select the original name listed in the Agent Managed view in the results pane. This entry has the original name before it was renamed.
3. Select **Delete** in the Actions pane located on the right side of the Operation Manager's console. This action removes the renamed server from the view.
4. Add the new server name by following the instructions in "Adding an IBM system that will be managed by the Operations Manager" on page 61.



---

## Appendix B. Troubleshooting

The topics in this section provide information to assist you with troubleshooting issues that you may have with the IBM Hardware Management Pack. The recommended actions often start with you verifying that you have performed certain tasks. The symptoms of a problem often provide a clue to the underlying issue.

---

### Troubleshooting errors returned from the IBM Power CIM Provider

This topic describes how to troubleshoot errors returned from the IBM Power CIM Provider.

There are two possible reasons why **Capping Capable** is reported as False:

- The system firmware is reporting that a platform or firmware subcomponent does not support power capping. A possible resolution would be to consult IBM power management guide to determine if there is a uEFI setting that can be set to activate the power capping capability.
- The system type does not support the power capping feature.

For more information about IBM power management, see the IBM Systems Director Active Energy Manager Information Center.

---

### Troubleshooting the installation of the IBM Power CIM Provider

The topics in this section describe how to troubleshoot the installation of the IBM Power CIM Provider. The first step in troubleshooting the installation of the IBM Power CIM Provider is to verify that the installation successfully finished.

For more information, see “Verifying an IBM Power CIM installation finished successfully.”

#### Verifying an IBM Power CIM installation finished successfully

The following procedure describes how to verify whether an installation of the IBM Power CIM Provider finished successfully.

## About this task

Perform the following steps from an Administrator Command window.

### Procedure

1. Execute the following commands:
  - a. `cimprovider -l -m IBMPowerCIM`  
The result of this command should be a line with the provider name (IBMPowerCIM) and a status of **OK**.
  - b. `cimcli ei -n root/ibmsd IBMPSG_AveragePowerUsageValue`
  - c. `cimcli ei -n root/ibmsd IBMPSG_AveragePowerUsageSensor`
  - d. `cimcli ei -n root/ibmsd IBMPSG_PowerCappingInformation`
2. Verify the output generated when these commands are run. The output should indicate appropriate numbers for the sensor readings and lower threshold values, and Pmin/Pmax for the PowerCappingInformation class. If a command indicates that it partially failed, the command to generate the appropriate numbers did not successfully run, therefore, the command run failed.
3. Optional: If any of the commands for verifying the IBM Power CIM Provider installation failed or provided some improper values, see “How to fix a failed IBM Power CIM Provider installation.”

## How to fix a failed IBM Power CIM Provider installation

The following procedure describes how to fix a failed IBM Power CIM Provider installation.

### About this task

If any of the commands for verifying the IBM Power CIM Provider installation failed or provided some improper values, complete the following steps:

### Procedure

1. Verify that the registry key exists and contains the appropriate values.  
The key is located in HKLM\SOFTWARE\IBM\System Management Integrations\IBM Power CIM Provider. It should contain a **REG\_SZ** parameter named *Path*, which lists the installation directory of the provider. This directory should be writeable.  
  
**Note:** On 64-bit machines, this key can be found in: HKLM\SOFTWARE\Wow6432Node\IBM\System Management Integrations\IBM Power CIM Provider.
2. In the installation directory, open the IBMPowerCIMRegistration.mof file and verify that the **Location** line lists the proper path: \IBMPowerCIM. The default installation path is %ProgramFiles%\IBM\IBM Power CIM Provider.



3. Select one of the following options:
  - Stop here if there are no reports of failure or improper values after verifying that the location line lists the proper path.
  - Complete steps 4 through 8 if the provider is still reporting failure or improper values.
4. Review the log files located in the installation directory. The file called `RegIBMPowerCIM.log` shows the results of the registration (and deregistration) scripts that are executed during the Windows Installer installation and uninstallation processes. If an error occurred while running these installation scripts, the results of that error is shown in the `RegIBMPowerCIM.log` file. There can be two possible causes:
  - **Response length = 256**  
The most common cause for this error is that SMBIOS Type 38 is not recognized on the system. This is because the system's firmware does not support SMBIOS Type 38 or the IPMI libraries are not properly recognizing it. Try restarting the cimserver (as noted below) or try restarting the computer.
  - **cmdComplete = false**  
Another common cause for this error is that the registry key path is incorrect.
5. Reinstall the IBM Power CIM Provider by using the provided installer and completing the following steps.
  - a. Remove the IBM Power CIM Provider by selecting **Uninstall** in **Add/Remove Programs** (Windows 2003) or **Programs and Features** (Windows 2008 and later).
  - b. Wait several minutes for the Director CIM server, *wmicimserver*, to come back online.
  - c. Reinstall the IBM Power CIM Provider using the provided installation file.
6. To manually reregister the IBM Power CIM Provider with the Director CIM server, enter the following commands from an Administrator Command window:
  - a. `cimprovider -r -m IBMPowerCIM`
  - b. `net stop wmicimserver`
  - c. `taskkill /F /IM wmicpa.exe`
  - d. `net start wmicimserver`
  - e. `mofcomp IBMPowerCIM.mof` (from the provider installation directory)
  - f. `mofcomp IBMPowerCIMRegistration.mof` (from the provider installation directory)
  - For optimal results, wait a few minutes between the `net start wmicimserver` command and the `mofcomp` command.

**Note:** *wmicimserver* sometimes takes a minute to become properly responsive to new providers being loaded.

7. Verify the server's firmware supports **SMBIOS Type 38**. If it does not, update to a firmware version that it does support. Computers with a Unified Extensible Firmware Interface should not be a problem.
8. In the registry key path `HKLM\SOFTWARE\[Wow6432Node]\IBM\System Management Integrations\IBM Power CIM Provider`:
  - a. Add a **REG\_SZ** named *Debug* and set the value to 1.
  - b. Uninstall and reinstall the IBM Power CIM Provider as described above. The logs are now more verbose, which may provide further insight into the issue.
9. Restart the server.

---

## How to remove an IBM Chassis in Network Devices Pending Management on Windows server 2012

The following procedure describes how to resolve the issue of an IBM BladeCenter or Flex system chassis being discovered but displaying in the **Network Devices Pending Management** view.

### About this task

If any of the IBM BladeCenter or Flex system chassis is displayed in the **Network Devices Pending Management** view, complete the following steps.

### Procedure

1. On a Windows machine of your management server(s), open the firewall settings, and find the inbound and outbound rules for starting with Operations Manager. Some rules may be disabled by default.
2. Enable the appropriate rules and then rerun the discovery rule, or wait for it to occur as a scheduled task on the SCOM Console. The network device you discovered is listed under **Network Devices** view and no longer under the **Network Devices Pending Management** view.

---

## How to fix a failed task of opening an IBM System Web Console on an SCOM Console using Windows Server 2012

When you try to run the **IBM IMM/AMM/CMM Web Console** task on a System Center Operations Manager Console on a managed system using Windows Server 2012, that has the SSL server for web console enabled and it fails, complete the following procedure to fix this problem. This is a Windows Server 2012 Internet Explorer security configuration problem.

## About this task

The following procedure describes how to change the Internet Explorer (IE) security configuration to allow IE to open the web console.

### Procedure

1. If your server is running Windows Server 2012, click **Server Manager** and then click **Configure this local server** to open the Local Server configuration page.
2. In the Properties area, next to IE Enhanced Security Configuration, click **On** to open the Internet Explorer Enhanced Security Configuration dialog box.
3. To use Internet Explorer Enhanced Configuration when members of the local Administrators group are logged in under Administrators, click **Off**. This allows you to use the Internet Explorer Enhanced Configuration when members of the local Administrators group are also logged in.
4. Click **OK** to apply the changes.



---

## Appendix C. Accessibility features

Accessibility features help users who have a physical disability, such as restricted mobility or limited vision, to use information technology products successfully.

IBM strives to provide products with usable access for everyone, regardless of age or ability.

The IBM Hardware Management Pack, version v5.5 supports the accessibility features of the system-management software in which are integrated. Refer to your system-management software documentation for specific information about accessibility features and keyboard navigation.

**Tip:** The IBM Hardware Management Pack, version v5.5 topic collection and its related publications are accessibility-enabled for the IBM Home Page Reader. You can operate all features using the keyboard instead of the mouse.

You can view the publications for IBM Hardware Management Pack, version v5.5 in Adobe Portable Document Format (PDF) using the Adobe Acrobat Reader. You can access the PDFs from the IBM Hardware Management Pack, version v5.5 download site.

### **IBM and accessibility**

See Human Ability and Accessibility Center Website for more information about the commitment that IBM has to accessibility.



---

## Notices

This information was developed for products and services offered in the U.S.A. IBM may not offer the products, services, or features discussed in this document in other countries.

Consult your local IBM representative for information on the products and services currently available in your area. Any reference to an IBM product, program, or service is not intended to state or imply that only that IBM product, program, or service may be used. Any functionally equivalent product, program, or service that does not infringe any IBM intellectual property right may be used instead. However, it is the user's responsibility to evaluate and verify the operation of any non-IBM product, program, or service.

IBM may have patents or pending patent applications covering subject matter described in this document. The furnishing of this document does not grant you any license to these patents. You can send license inquiries, in writing, to:

IBM Director of Licensing  
IBM Corporation  
North Castle Drive  
Armonk, NY 10504-1785  
U.S.A.

INTERNATIONAL BUSINESS MACHINES CORPORATION PROVIDES THIS PUBLICATION "AS IS" WITHOUT WARRANTY OF ANY KIND, EITHER EXPRESS OR IMPLIED, INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF NON-INFRINGEMENT, MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. Some states do not allow disclaimer of express or implied warranties in certain transactions, therefore, this statement may not apply to you.

This information could include technical inaccuracies or typographical errors. Changes are periodically made to the information herein; these changes are incorporated in new editions of the publication. IBM may make improvements and/or changes in the product(s) and/or the program(s) described in this publication at any time without notice.

Any references in this information to non-IBM web sites are provided for convenience only and do not in any manner serve as an endorsement of those web sites. The materials at those Web sites are not part of the materials for this IBM product, and use of those web sites is at your own risk.

IBM may use or distribute any of the information you supply in any way it believes appropriate without incurring any obligation to you.

---

## Trademarks

IBM, the IBM logo, and [ibm.com](http://www.ibm.com)<sup>®</sup> are trademarks or registered trademarks of International Business Machines Corporation in the United States, other countries, or both. If these and other IBM trademarked terms are marked on their first occurrence in this information with a trademark symbol (<sup>®</sup> or <sup>™</sup>), these symbols indicate U.S. registered or common law trademarks owned by IBM at the time this information was published.

Such trademarks may also be registered or common law trademarks in other countries. A current list of IBM trademarks is available on the web at Copyright and trademark information at <http://www.ibm.com/legal/copytrade.shtml>.

Adobe and PostScript are either registered trademarks or trademarks of Adobe Systems Incorporated in the United States, other countries, or both.

Cell Broadband Engine is a trademark of Sony Computer Entertainment, Inc., in the United States, other countries, or both and is used under license therefrom.

Intel, Intel Xeon, Itanium, and Pentium are trademarks or registered trademarks of Intel Corporation or its subsidiaries in the United States and other countries.

Java<sup>™</sup> and all Java-based trademarks are trademarks of Sun Microsystems, Inc., in the United States, other countries, or both.

Linux is a registered trademark of Linus Torvalds in the United States, other countries, or both.

Microsoft, Windows, and Windows NT are trademarks of Microsoft Corporation in the United States, other countries, or both.

UNIX is a registered trademark of The Open Group in the United States and other countries.

Other company, product, or service names may be trademarks or service marks of others.

---

## Important notes

View important assumptions about terminology and claims.



Processor speed indicates the internal clock speed of the microprocessor; other factors also affect application performance.

CD or DVD drive speed is the variable read rate. Actual speeds vary and are often less than the possible maximum.

When referring to processor storage, real and virtual storage, or channel volume, KB stands for 1024 bytes, MB stands for 1,048,576 bytes, and GB stands for 1,073,741,824 bytes.

When referring to hard disk drive capacity or communications volume, MB stands for 1,000,000 bytes, and GB stands for 1,000,000,000 bytes. Total user-accessible capacity can vary depending on operating environments.

Maximum internal hard disk drive capacities assume the replacement of any standard hard disk drives and population of all hard disk drive bays with the largest currently supported drives that are available from IBM.

Maximum memory might require replacement of the standard memory with an optional memory module.

IBM makes no representation or warranties regarding non-IBM products and services that are ServerProven, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. These products are offered and warranted solely by third parties.

IBM makes no representations or warranties with respect to non-IBM products. Support (if any) for the non-IBM products is provided by the third party, not IBM.

Some software might differ from its retail version (if available) and might not include user manuals or all program functionality.



---

# Index

## A

About this publication ix  
Accessibility features 135  
adding an IBM system 63  
adding an IBM system to be managed by the Operations Manager 61  
additional configuration requirements 11  
Adobe Acrobat Reader xi

## B

Baseboard Management Controller 13  
BladeCenter 4, 126, 127  
BladeCenter chassis 7

## C

configuring IBM Flex System Chassis SNMP settings 45  
conventions and terminology ix  
creating an SNMPv3 user account 49

## D

deleting the IBM Hardware Management Packs 29  
determining the cause of an error 123  
discovering an IBM Flex System in Operations Manager 2007 50  
discovering an IBM Flex System in Operations Manager 2012 51  
discovering an IBM FSM system 109  
discovering the Flex System OOB-IB Reflection 100

## E

enabling power capping 91

## F

Flex System Chassis Web Console 106  
Flex System OOB-IB Reflection 100  
Flex system remote power on and off 102  
FSM Web Console 111

## H

Health Explorer 75  
how to check software dependencies on the remote computer 61  
how to fix a failed task of opening an IBM System Web Console 132

## I

IBM BladeCenter 4, 5  
IBM Director Core Services 4  
IBM FSM system 109  
IBM Hardware Management Pack 1, 3, 4, 26, 28, 31  
IBM Hardware Management Pack, installation 17  
IBM Power CIM Provider 27, 30, 129  
IBM ServerProven sites xii  
IBM System x Integration Offerings site xi  
IBM System x Power Data Chart 99  
IBM systems 4  
IBM Systems Director Agent 12  
IBM Systems Management site xii  
IBM Systems Technical support site xi  
important notes 138  
imported IBM Hardware Management Packs 25  
information resources xi  
installation 17  
installation requirements 18  
installing IBM Power CIM Provider 27  
Integrated Management Module 13  
Integrated RAID 14

## K

key features 1  
Knowledge pages 77

## L

launching the FSM Web Console 111  
launching the IBM Flex System Chassis Web Console 106  
locating hardware errors 75

## M

managed systems, operating systems 11  
management concepts 4  
management server 26  
management servers 11  
management servers, operating systems 10  
MegaRAID 14  
Microsoft System Center Operations Manager 3, 4  
Microsoft System Center Operations Manager site xii  
monitoring the health of systems, hardware components, and other targets 72

## N

notices 137

## O

Operations Manager 53  
Operations Manager, supported versions 10

## P

PDF files xi  
Platform Agent 4  
Power Data Chart 99  
power monitoring, supported configurations for managed systems 15  
premium features 1  
product information 1

## R

rediscovering a renamed server 127  
rediscovering all BladeCenters 126  
reinstalling 31  
Remote Power On using the server name 84  
remote shut down of the operating system 81  
Remote Supervisor Adapter-II 13  
removing a discovered BladeCenter chassis 44  
removing a discovered IBM Flex System chassis 52  
removing an IBM Chassis 132  
RSA-II 13

## S

ServeRaid 15  
ServeRAID-BR/IR 14  
ServeRAID-MR 14  
setting power capping 91  
setting predictive failure alert policy 97  
setting the power threshold 86  
SNMPv1 Agent 48  
SNMPv3 Agent 49  
supported configurations 5, 12, 15  
supported configurations, managed systems 11  
supported configurations, management servers 10  
supported IBM Flex System chassis 7  
supported operating systems 5  
supported servers 5  
supported systems 5

## T

trademarks 138  
Trial license 2  
trial period 2  
troubleshooting 129

troubleshooting IBM Power CIM  
Provider 129

## U

uninstalling 28  
uninstalling IBM Hardware Management  
Pack 30  
using Flex system remote power on and  
off 102  
using Health Explorer to identify and  
resolve problems 75  
using the Operations Manager  
Console 53

## V

verifying the IBM Power CIM Provider  
installation 129  
viewing alerts 74  
viewing hardware errors 75  
viewing inventory 72

## W

web resources xi

---

## Readers' Comments — We'd Like to Hear from You

IBM System x  
IBM Hardware Management Pack for  
Microsoft System Center Operations Manager  
Installation and User's Guide  
Version 5.5

We appreciate your comments about this publication. Please comment on specific errors or omissions, accuracy, organization, subject matter, or completeness of this book. The comments you send should pertain to only the information in this manual or product and the way in which the information is presented.

For technical questions and information about products and prices, please contact your IBM branch office, your IBM business partner, or your authorized remarketer.

When you send comments to IBM, you grant IBM a nonexclusive right to use or distribute your comments in any way it believes appropriate without incurring any obligation to you. IBM or any other organizations will only use the personal information that you supply to contact you about the issues that you state on this form.

Comments:

Thank you for your support.

Send your comments to the address on the reverse side of this form.

If you would like a response from IBM, please fill in the following information:

\_\_\_\_\_

Name

\_\_\_\_\_

Address

\_\_\_\_\_

Company or Organization

\_\_\_\_\_

Phone No.

\_\_\_\_\_

Email address



Fold and Tape

Please do not staple

Fold and Tape



NO POSTAGE  
NECESSARY  
IF MAILED IN THE  
UNITED STATES

# BUSINESS REPLY MAIL

FIRST-CLASS MAIL PERMIT NO. 40 ARMONK, NEW YORK

POSTAGE WILL BE PAID BY ADDRESSEE

International  
Business Machines Corporation  
PO Box 12195  
Research Triangle Park  
NC  
U.S.A. 27709-9990



Fold and Tape

Please do not staple

Fold and Tape





Printed in USA